
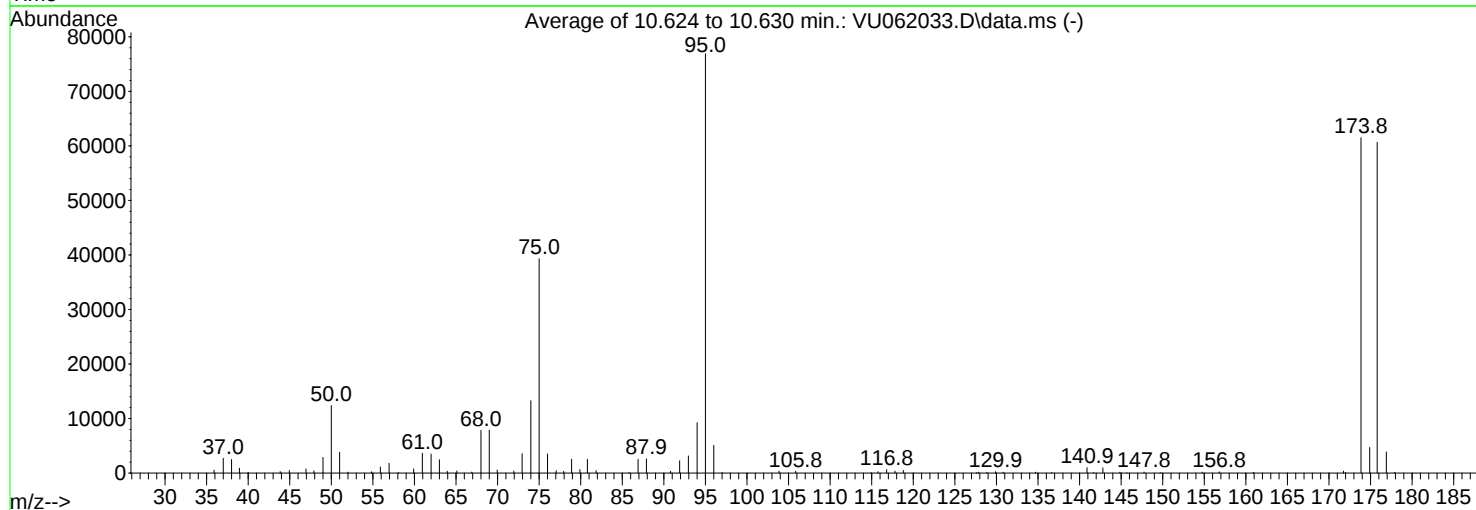


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112624\
Data File : VU062033.D
Acq On : 26 Nov 2024 08:07
Operator : MD/SY
Sample : BFB037
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB037

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR112024WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Nov 25 01:25:39 2024

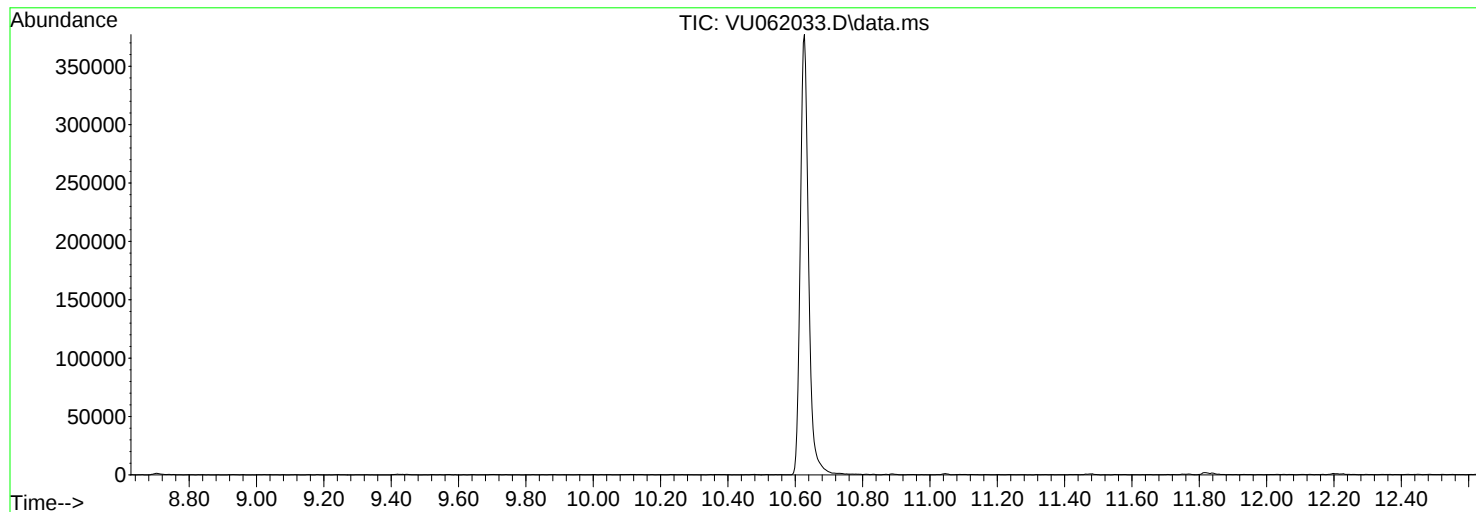

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	12393	PASS
75	95	30	80	51.1	39304	PASS
95	95	100	100	100.0	76907	PASS
96	95	5	9	6.6	5097	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.0	61507	PASS
175	174	5	9	7.6	4690	PASS
176	174	95	101	98.6	60664	PASS
177	176	5	9	6.4	3886	PASS

m/z	Abundance
43.80	115.0

Instrument :
MSVOA_U
ClientSampleId :
BFB037

m/z	Abundance
35.90	567.0
37.00	2901.0
38.00	2635.0
39.00	951.0
40.00	110.0
43.90	427.0
45.00	517.0
46.90	822.0
47.90	490.0
49.00	2919.0
50.00	12838.0
51.00	3851.0
51.90	209.0
54.80	274.0
55.90	1135.0
56.90	1757.0
59.90	764.0
61.00	3699.0
62.00	3552.0
63.00	2517.0
63.90	334.0
65.10	458.0
67.00	221.0
68.00	7955.0
69.00	8091.0
69.90	503.0
71.90	378.0
73.00	3507.0
74.00	13403.0
75.00	40080.0
76.00	3629.0
77.00	378.0
78.00	312.0
78.90	2552.0
79.90	655.0
80.80	2765.0
81.80	464.0
85.80	153.0
86.90	2602.0
87.90	2650.0
90.80	307.0
91.90	2300.0
92.90	3237.0
94.00	9571.0
95.00	78072.0
96.00	5441.0
97.00	155.0
103.80	385.0
105.90	323.0
115.80	279.0
116.70	639.0
117.80	401.0
118.80	538.0
127.60	244.0
128.80	171.0
129.90	266.0
130.80	182.0
134.70	158.0
136.70	146.0
140.90	1050.0
141.70	145.0
142.80	899.0
144.80	162.0
147.70	206.0
149.70	105.0
154.70	176.0
156.80	205.0
160.90	127.0
171.80	422.0
173.90	60864.0
174.90	4867.0
175.80	59984.0
176.90	4049.0
177.90	119.0

Instrument :
MSVOA_U
ClientSampleId :
BFB037

m/z	Abundance
35.90	591.0
37.00	2782.0
38.00	2567.0
39.00	913.0
40.00	132.0
43.90	406.0
44.90	513.0
47.00	776.0
47.90	411.0
49.00	2989.0
50.00	12698.0
51.00	3930.0
52.00	170.0
54.80	258.0
55.90	1155.0
56.90	1841.0
58.10	114.0
59.90	781.0
61.00	3750.0
62.00	3573.0
63.00	2484.0
63.90	342.0
65.10	400.0
66.90	186.0
68.00	8138.0
69.00	8104.0
70.00	578.0
72.00	376.0
73.00	3711.0
74.00	13623.0
75.00	40632.0
76.00	3644.0
77.10	360.0
77.90	336.0
78.90	2687.0
79.90	666.0
80.80	2595.0
81.80	458.0
85.80	124.0
86.90	2559.0
87.90	2655.0
90.80	317.0
91.90	2311.0
92.90	3215.0
94.00	9525.0
95.00	79128.0
96.00	5245.0
97.00	119.0
103.80	337.0
105.80	371.0
115.70	242.0
116.80	636.0
117.80	405.0
118.80	517.0
127.90	239.0
128.80	156.0
129.90	272.0
130.80	176.0
134.70	170.0
136.60	140.0
140.90	1025.0
141.70	126.0
142.80	1008.0
144.80	155.0
147.70	215.0
149.70	104.0
154.70	176.0
156.80	231.0
160.90	133.0
171.80	370.0
173.80	63288.0
174.90	4884.0
175.80	62704.0
176.90	3997.0
177.90	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB037

m/z	Abundance
35.90	487.0
37.00	2471.0
38.00	2256.0
38.90	834.0
40.00	134.0
43.90	367.0
44.90	416.0
47.00	688.0
47.90	363.0
49.00	2705.0
50.00	11643.0
51.00	3680.0
52.10	149.0
54.90	214.0
55.90	1054.0
57.00	1777.0
58.10	112.0
59.90	729.0
60.90	3483.0
62.00	3366.0
63.00	2373.0
64.00	350.0
65.10	330.0
66.80	164.0
68.00	7477.0
69.00	7429.0
70.00	579.0
71.90	358.0
72.90	3478.0
74.00	12810.0
75.00	37200.0
76.00	3231.0
76.90	315.0
77.10	313.0
77.90	326.0
78.90	2421.0
79.90	641.0
80.80	2187.0
81.90	463.0
86.90	2446.0
87.90	2496.0
90.80	335.0
91.90	2158.0
93.00	2987.0
94.00	8626.0
95.00	73520.0
96.00	4606.0
103.90	333.0
105.80	375.0
114.90	103.0
115.70	235.0
116.90	617.0
117.80	339.0
118.80	401.0
127.80	265.0
128.90	109.0
129.90	264.0
130.80	154.0
134.70	170.0
136.60	124.0
140.90	922.0
142.80	994.0
144.90	162.0
145.70	142.0
147.80	192.0
154.80	168.0
156.80	211.0
160.90	135.0
171.70	333.0
172.00	333.0
173.80	60368.0
174.90	4319.0
175.80	59304.0
176.90	3613.0
177.90	124.0

Instrument :
MSVOA_U
ClientSampleId :
BFB037