
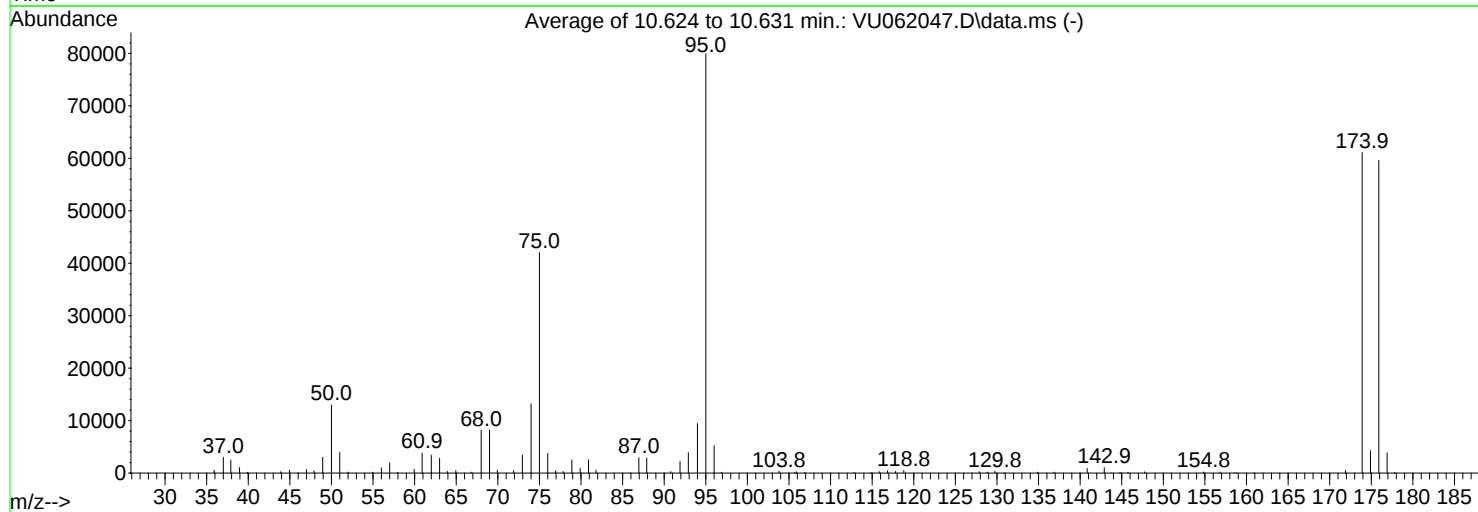


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112724\
Data File : VU062047.D
Acq On : 27 Nov 2024 08:06
Operator : MD/SY
Sample : BFB038
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB038

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR112024WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Nov 28 02:06:22 2024

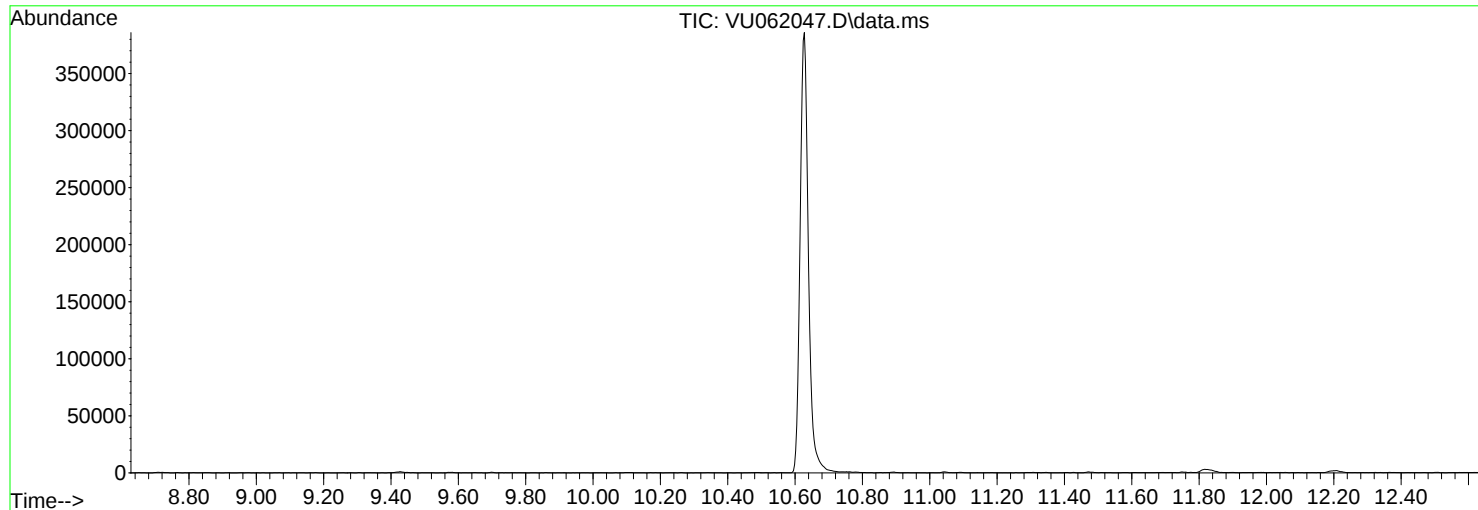

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	12990	PASS
75	95	30	80	52.6	42035	PASS
95	95	100	100	100.0	79939	PASS
96	95	5	9	6.5	5217	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.4	61109	PASS
175	174	5	9	7.0	4260	PASS
176	174	95	101	97.5	59595	PASS
177	176	5	9	6.5	3875	PASS

m/z	Abundance
43.80	144.0

Instrument :
MSVOA_U
ClientSampleId :
BFB038

m/z	Abundance
35.90	588.0
37.00	3183.0
37.90	2565.0
38.90	1114.0
39.90	122.0
44.00	396.0
44.90	590.0
47.00	734.0
47.90	479.0
49.00	3111.0
50.00	13284.0
51.00	4078.0
52.00	161.0
55.00	211.0
56.00	1066.0
57.00	1967.0
57.90	127.0
59.90	777.0
60.90	3895.0
62.00	3469.0
63.00	2965.0
63.90	324.0
64.90	494.0
66.80	135.0
68.00	8483.0
69.00	8297.0
69.90	572.0
71.90	455.0
72.90	3441.0
74.00	13443.0
75.00	42976.0
76.00	3860.0
76.90	529.0
77.80	303.0
78.90	2673.0
79.90	972.0
80.90	2507.0
81.80	542.0
85.90	112.0
86.90	2956.0
87.90	3035.0
90.80	289.0
91.90	2298.0
92.90	4005.0
94.00	9712.0
95.00	80440.0
96.00	5326.0
96.90	196.0
103.80	363.0
105.70	385.0
106.90	100.0
114.90	113.0
115.80	287.0
116.90	464.0
117.80	313.0
118.80	469.0
127.90	345.0
128.80	184.0
129.70	336.0
130.90	123.0
134.90	150.0
136.90	172.0
140.90	957.0
142.90	1052.0
144.90	126.0
145.80	167.0
147.70	260.0
154.80	240.0
156.80	142.0
158.60	119.0
160.90	109.0
171.90	501.0
173.90	60528.0
174.90	4231.0
175.90	59104.0
176.90	3965.0
177.80	145.0

Instrument :
MSVOA_U
ClientSampleId :
BFB038

m/z	Abundance
35.90	575.0
37.00	3119.0
37.90	2566.0
38.90	1082.0
39.90	142.0
44.00	413.0
44.90	550.0
47.00	683.0
47.90	453.0
49.00	3103.0
50.00	13357.0
51.00	4073.0
52.00	222.0
55.00	189.0
56.00	1026.0
57.00	2017.0
57.90	136.0
60.00	747.0
60.90	3961.0
62.00	3477.0
63.00	2924.0
63.90	331.0
65.00	469.0
66.80	184.0
68.00	8517.0
69.00	8451.0
69.90	563.0
71.90	496.0
73.00	3536.0
74.00	13468.0
75.00	43152.0
76.00	3876.0
76.90	448.0
77.90	298.0
78.90	2546.0
79.90	896.0
80.90	2620.0
81.80	543.0
87.00	2926.0
87.90	2912.0
90.80	286.0
91.90	2310.0
92.90	3960.0
94.00	9755.0
95.00	82400.0
96.00	5355.0
96.90	172.0
103.80	400.0
105.90	382.0
106.90	127.0
112.80	114.0
114.80	112.0
115.90	289.0
116.80	485.0
117.80	308.0
118.80	518.0
127.80	265.0
128.80	211.0
129.80	391.0
130.80	104.0
134.90	177.0
136.80	183.0
140.80	877.0
142.90	1035.0
144.80	127.0
145.70	159.0
147.70	231.0
154.80	238.0
156.80	203.0
158.60	117.0
171.90	536.0
173.90	62904.0
174.90	4411.0
175.90	61536.0
176.90	4009.0
177.80	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB038

m/z	Abundance
35.90	523.0
37.00	2738.0
37.90	2316.0
39.00	959.0
39.90	150.0
44.00	423.0
45.00	475.0
46.00	109.0
47.00	564.0
47.90	407.0
48.90	2811.0
50.00	12329.0
51.00	3723.0
52.00	233.0
54.90	150.0
56.00	897.0
57.00	1898.0
58.00	121.0
60.00	689.0
60.90	3621.0
62.00	3296.0
63.00	2656.0
64.00	313.0
65.00	478.0
66.80	198.0
68.00	7557.0
69.00	7877.0
70.00	555.0
71.90	518.0
73.00	3359.0
74.00	12721.0
75.00	39976.0
76.00	3506.0
77.00	353.0
77.90	342.0
78.90	2214.0
79.90	769.0
80.90	2453.0
81.80	533.0
87.00	2923.0
87.90	2638.0
90.80	274.0
91.90	2077.0
92.90	3734.0
94.00	8868.0
95.00	76976.0
96.00	4971.0
96.90	140.0
103.80	393.0
105.90	361.0
106.90	122.0
112.80	118.0
115.90	310.0
116.80	466.0
117.80	278.0
118.80	489.0
127.80	215.0
128.80	179.0
129.80	394.0
134.80	204.0
136.80	171.0
140.80	792.0
142.90	1017.0
143.80	104.0
144.70	171.0
145.70	160.0
147.80	213.0
154.90	210.0
156.80	231.0
158.80	118.0
171.90	489.0
173.90	59896.0
174.90	4137.0
175.90	58144.0
176.90	3651.0
177.80	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB038