

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112824\
 Data File : VU062061.D
 Acq On : 27 Nov 2024 19:06
 Operator : MD/SY
 Sample : VU1128MBL01
 Misc : 5.00g/5mL/100ul/5ml/MSVOA_U/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Nov 28 01:17:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112724WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Nov 28 01:06:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.239	114	177164	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	163624	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	73889	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	57766	47.060	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	94.120%
7) Chloroethane-d5	1.904	69	43252	48.890	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	97.780%
11) 1,1-Dichloroethene-d2	2.560	63	83465	35.863	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.720%
21) 2-Butanone-d5	4.618	46	87385	104.760	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	104.760%
24) Chloroform-d	5.052	84	118861	46.395	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.780%
26) 1,2-Dichloroethane-d4	5.689	65	77918	47.673	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.340%
32) Benzene-d6	5.718	84	232232	49.633	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.260%
36) 1,2-Dichloropropane-d6	6.679	67	74675	50.785	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.580%
41) Toluene-d8	7.888	98	211826	48.903	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.800%
43) trans-1,3-Dichloroprop...	8.171	79	35279	48.009	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.020%
47) 2-Hexanone-d5	8.627	63	58061	104.824	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	104.820%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	105960	49.519	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	99.040%
66) 1,2-Dichlorobenzene-d4	12.184	152	77068	53.019	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.040%
Target Compounds						
37) 1,2-Dichloropropane	6.682	63	7871	6.109	ug/L	Qvalue # 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112824\
Data File : VU062061.D
Acq On : 27 Nov 2024 19:06
Operator : MD/SY
Sample : VU1128MBL01
Misc : 5.00g/5mL/100ul/5mL/MSVOA_U/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Nov 28 01:17:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112724WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Nov 28 01:06:41 2024
Response via : Initial Calibration

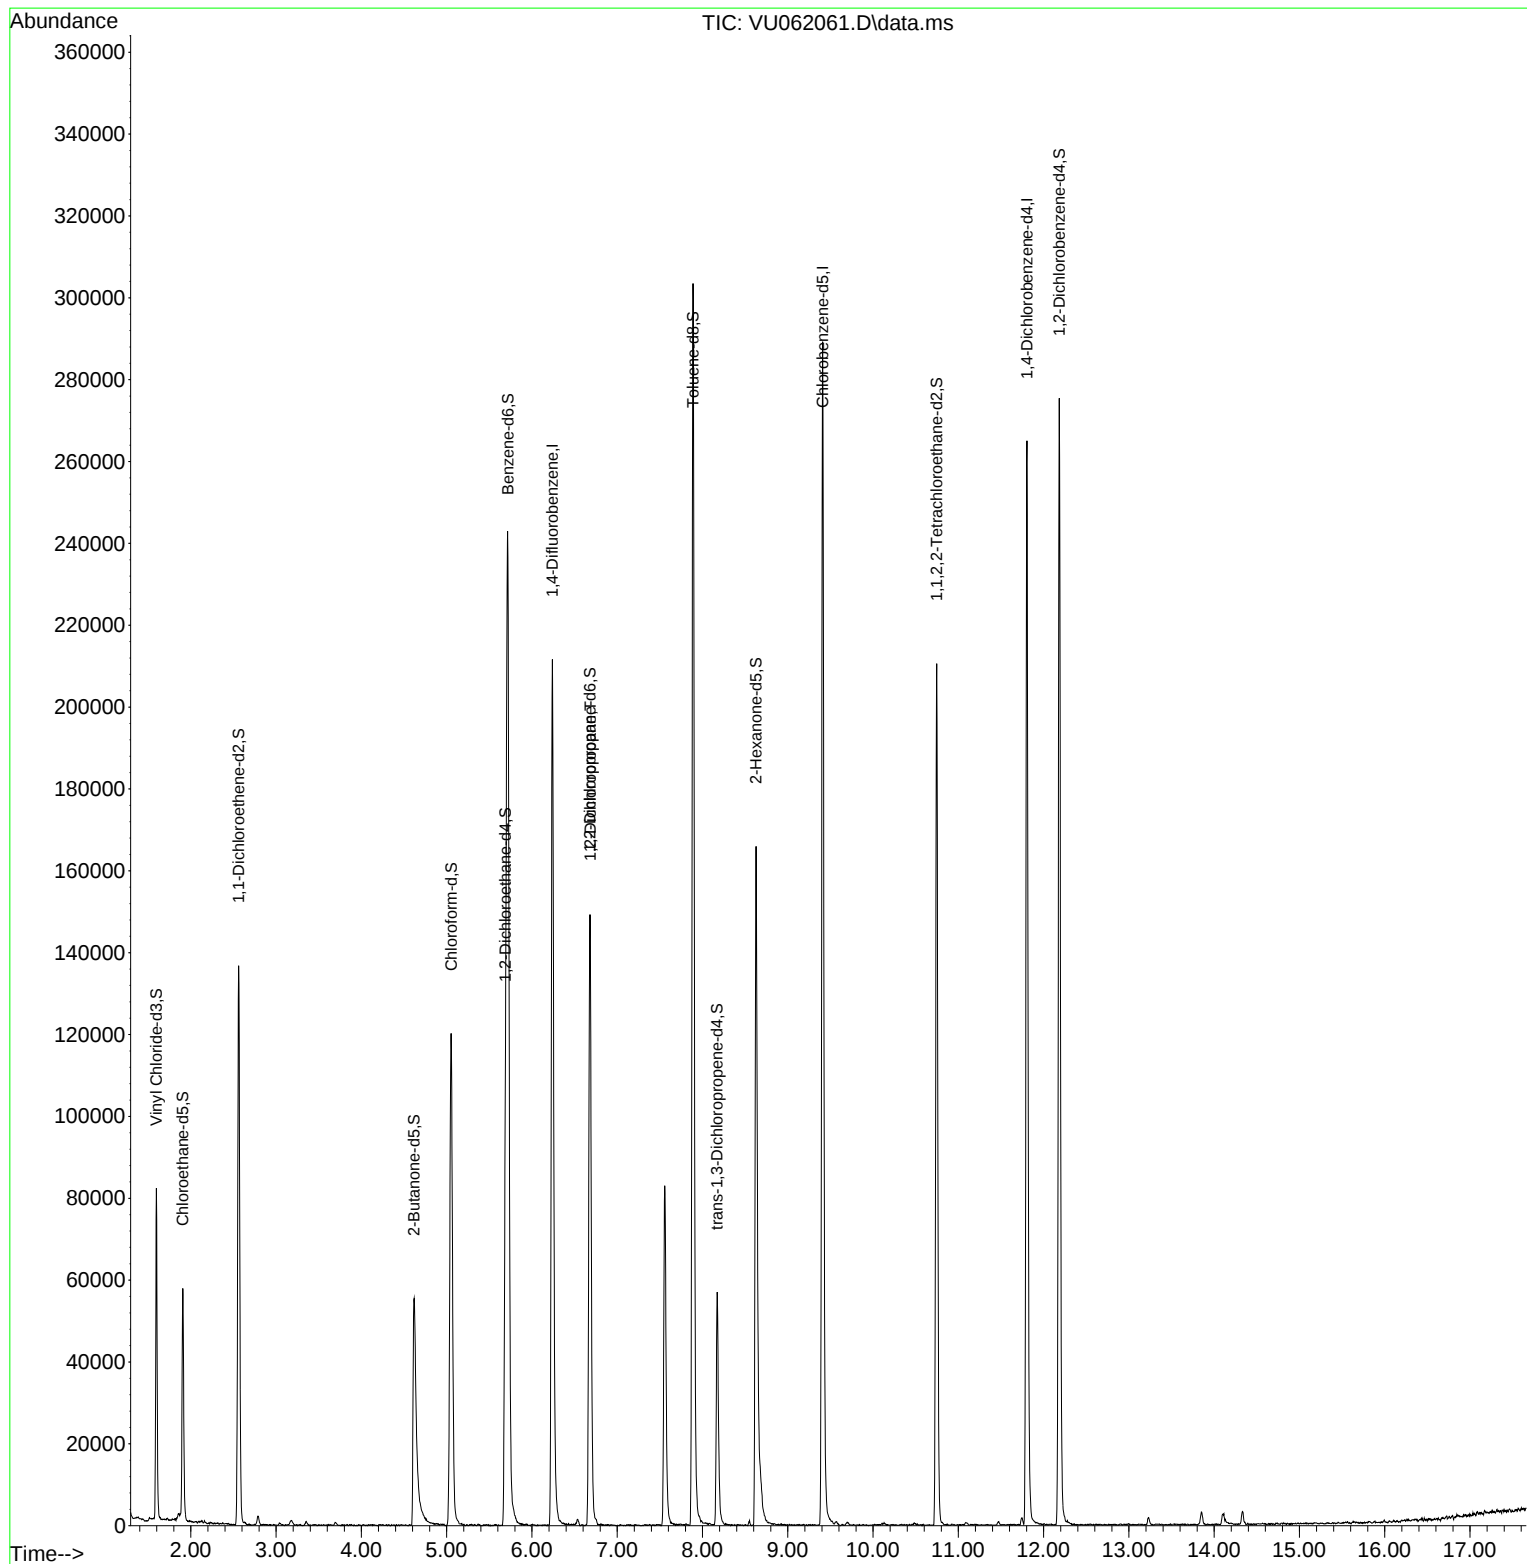

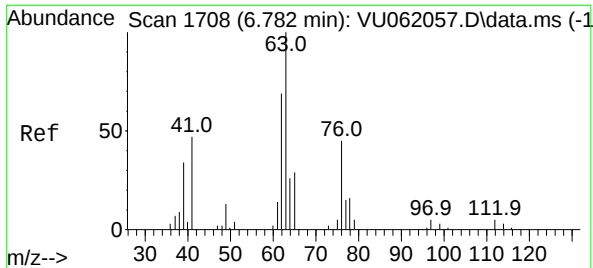

#37
1,2-Dichloropropane
Concen: 6.109 ug/L
RT: 6.682 min Scan# 1
Delta R.T. -0.100 min
Lab File: VU062061.D
Acq: 27 Nov 2024 19:06

Instrument :
MSVOA_U
ClientSampleId :

Tgt Ion: 63 Resp: 7871
Ion Ratio Lower Upper
63 100
112 0.0 3.1 4.7#

