

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112824\
 Data File : VU062062.D
 Acq On : 27 Nov 2024 19:30
 Operator : MD/SY
 Sample : VU1128WBL01
 Misc : 5mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Nov 28 01:17:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112724WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Nov 28 01:06:41 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		6.238	114	160881	50.000	ug/L	0.00
28) Chlorobenzene-d5		9.409	117	150034	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.804	152	66916	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.596	65	56842	50.994	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	101.980%	
7) Chloroethane-d5		1.907	69	43276	53.868	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	107.740%	
11) 1,1-Dichloroethene-d2		2.560	63	82134	38.862	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.720%	
21) 2-Butanone-d5		4.618	46	85729	113.177	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	113.180%	
24) Chloroform-d		5.052	84	121015	52.016	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.040%	
26) 1,2-Dichloroethane-d4		5.692	65	81856	55.151	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	110.300%	
32) Benzene-d6		5.718	84	233794	54.493	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	108.980%	
36) 1,2-Dichloropropane-d6		6.679	67	73755	54.703	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	109.400%	
41) Toluene-d8		7.888	98	208839	52.581	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.160%	
43) trans-1,3-Dichloroprop...		8.171	79	36074	53.537	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	107.080%	
47) 2-Hexanone-d5		8.627	63	58361	114.909	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	114.910%	
56) 1,1,2,2-Tetrachloroeth...		10.746	84	107730	54.906	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	109.820%	
66) 1,2-Dichlorobenzene-d4		12.184	152	76400	58.037	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	116.080%	
Target Compounds							Qvalue
37) 1,2-Dichloropropane		6.682	63	8294	7.021	ug/L	# 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112824\
Data File : VU062062.D
Acq On : 27 Nov 2024 19:30
Operator : MD/SY
Sample : VU1128WBL01
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Nov 28 01:17:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112724WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Nov 28 01:06:41 2024
Response via : Initial Calibration

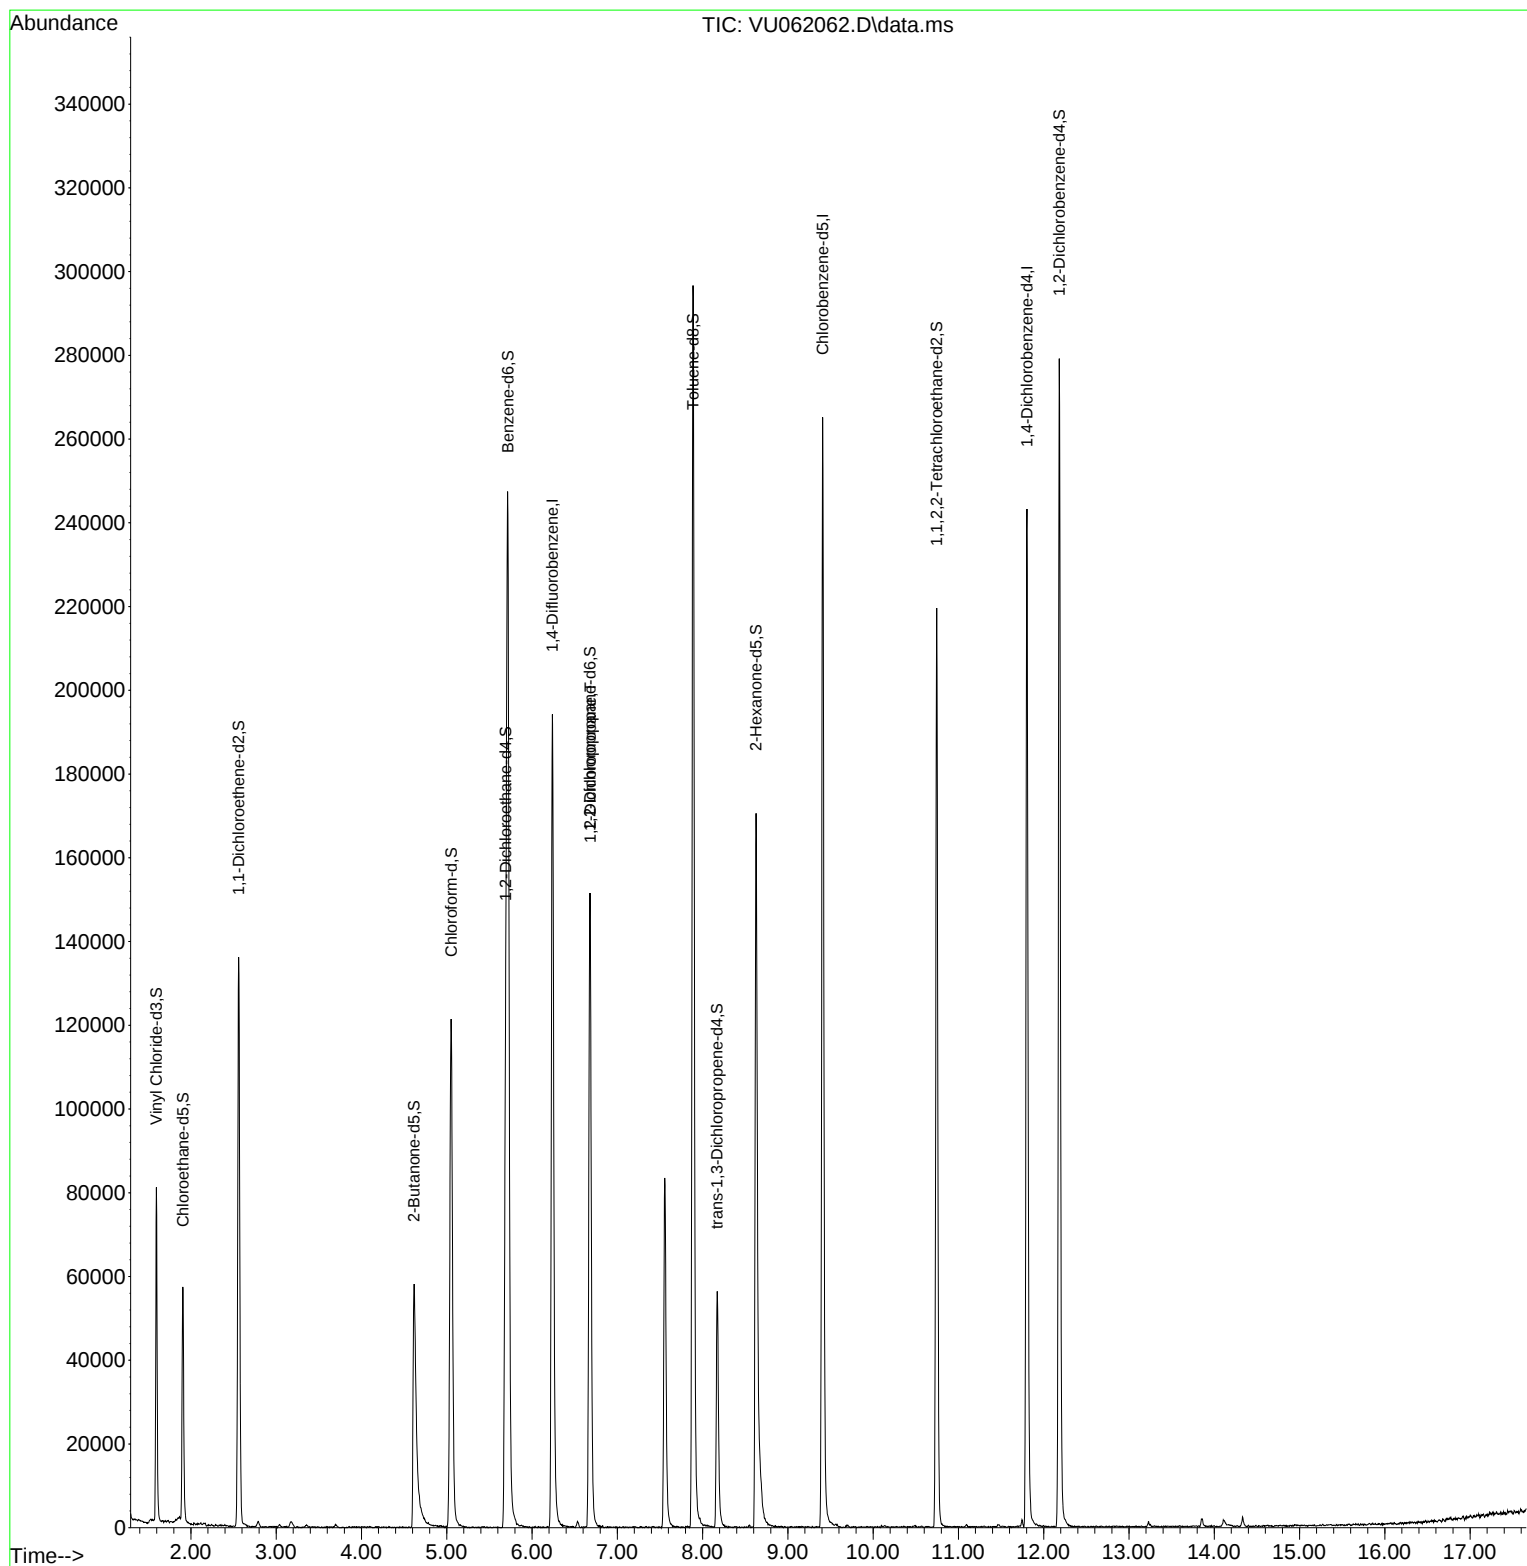

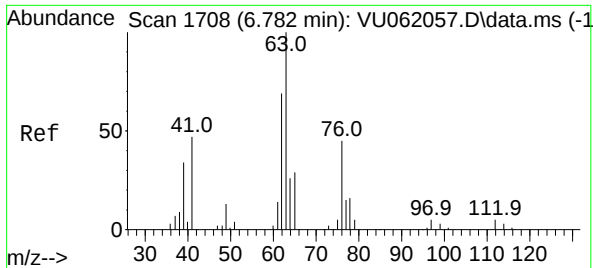

#37
1,2-Dichloropropane
Concen: 7.021 ug/L
RT: 6.682 min Scan# 1
Delta R.T. -0.100 min
Lab File: VU062062.D
Acq: 27 Nov 2024 19:30

Instrument :
MSVOA_U
ClientSampleId :

Tgt Ion: 63 Resp: 8294
Ion Ratio Lower Upper
63 100
112 0.0 3.1 4.7#

