
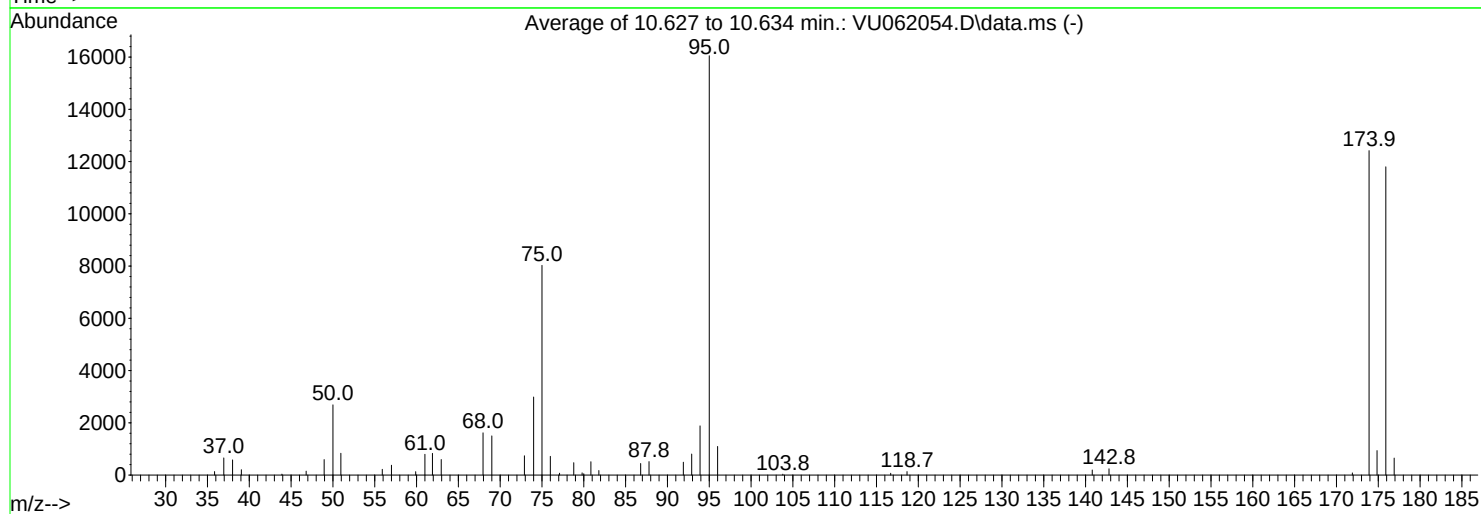


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112824\
Data File : VU062054.D
Acq On : 27 Nov 2024 14:02
Operator : MD/SY
Sample : BFB080
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB080

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112724WMA.M
Title : VOC Analysis
Last Update : Thu Nov 28 01:06:41 2024

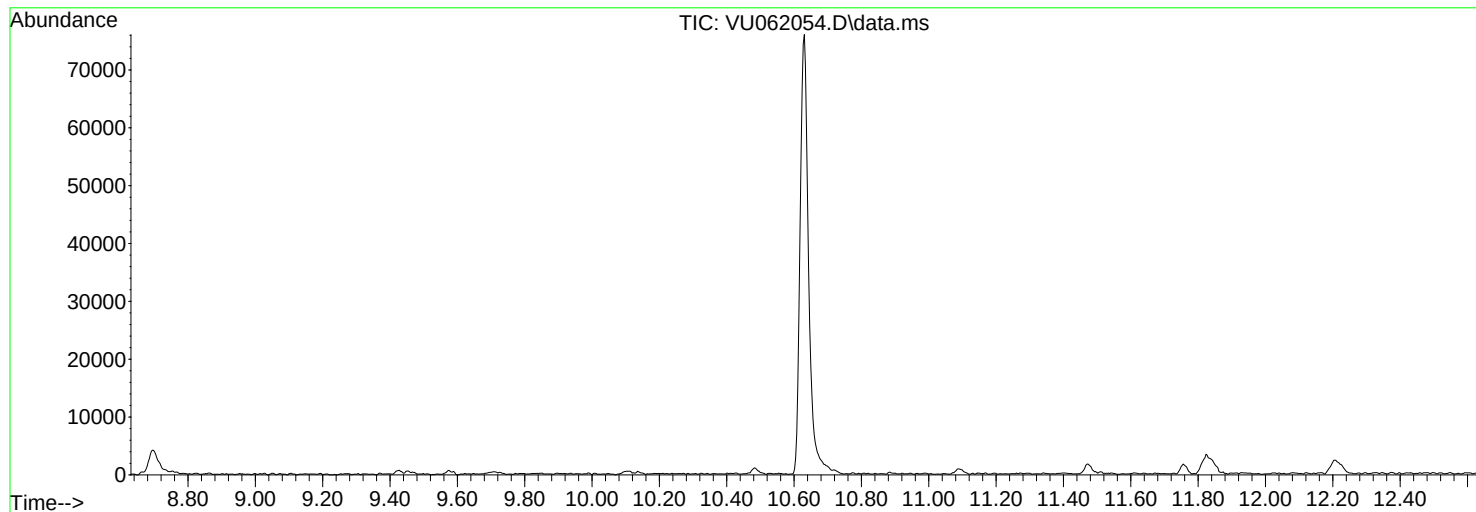

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2893

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	2688	PASS
75	95	30	80	50.0	8027	PASS
95	95	100	100	100.0	16051	PASS
96	95	5	9	6.8	1095	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.4	12418	PASS
175	174	5	9	7.6	938	PASS
176	174	95	101	95.0	11800	PASS
177	176	5	9	5.5	651	PASS

m/z	Abundance
43.90	158.0

Instrument :
MSVOA_U
ClientSampleId :
BFB080

m/z	Abundance
35.80	152.0
36.90	729.0
38.00	602.0
39.10	210.0
43.90	196.0
46.80	143.0
48.90	610.0
50.00	2692.0
50.90	857.0
55.90	232.0
57.00	340.0
59.90	137.0
61.00	797.0
61.90	864.0
63.00	578.0
67.90	1678.0
69.00	1550.0
72.90	760.0
74.00	2858.0
75.00	8209.0
76.00	706.0
78.80	524.0
79.80	115.0
80.80	557.0
81.80	185.0
86.80	472.0
87.80	501.0
91.90	482.0
92.90	845.0
93.90	1995.0
95.00	16300.0
96.00	1181.0
103.80	106.0
116.70	105.0
118.70	130.0
140.70	238.0
142.80	258.0
173.90	12002.0
174.80	949.0
175.90	11922.0
176.90	739.0

Instrument :
MSVOA_U
ClientSampleId :
BFB080

m/z	Abundance
35.90	141.0
37.00	660.0
38.00	609.0
39.00	204.0
44.00	188.0
46.80	151.0
49.00	615.0
50.00	2771.0
51.00	849.0
55.90	219.0
57.00	386.0
59.90	136.0
61.00	818.0
61.90	880.0
63.00	621.0
68.00	1671.0
69.00	1517.0
72.90	765.0
74.00	3141.0
75.00	8232.0
76.00	741.0
77.10	110.0
78.80	492.0
79.80	141.0
80.80	518.0
81.80	189.0
86.80	443.0
87.80	512.0
91.90	514.0
92.90	845.0
93.90	1909.0
95.00	16584.0
96.00	1141.0
116.70	105.0
118.60	145.0
140.80	179.0
142.80	257.0
171.90	114.0
173.90	12886.0
174.80	949.0
175.90	12093.0
176.90	651.0

Instrument :
MSVOA_U
ClientSampleId :
BFB080

m/z	Abundance
35.90	108.0
37.00	580.0
38.00	533.0
39.00	201.0
43.90	197.0
46.80	155.0
49.00	558.0
50.00	2602.0
51.00	800.0
55.90	209.0
57.00	402.0
59.90	120.0
61.00	771.0
61.90	748.0
62.90	585.0
68.00	1503.0
69.00	1433.0
72.90	688.0
74.00	2965.0
75.00	7639.0
76.00	701.0
77.10	102.0
78.80	407.0
80.00	152.0
80.90	459.0
81.80	152.0
86.80	411.0
87.80	534.0
91.90	479.0
92.90	725.0
93.90	1745.0
95.00	15268.0
96.00	964.0
118.60	127.0
140.90	167.0
142.80	206.0
171.90	135.0
173.90	12367.0
174.90	916.0
175.90	11384.0
176.90	564.0

Instrument :
MSVOA_U
ClientSampleId :
BFB080