


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120224\
Data File : VU062066.D
Acq On : 02 Dec 2024 08:24
Operator : MD/SY
Sample : BFB039
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB039

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR112024WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Dec 03 00:21:51 2024

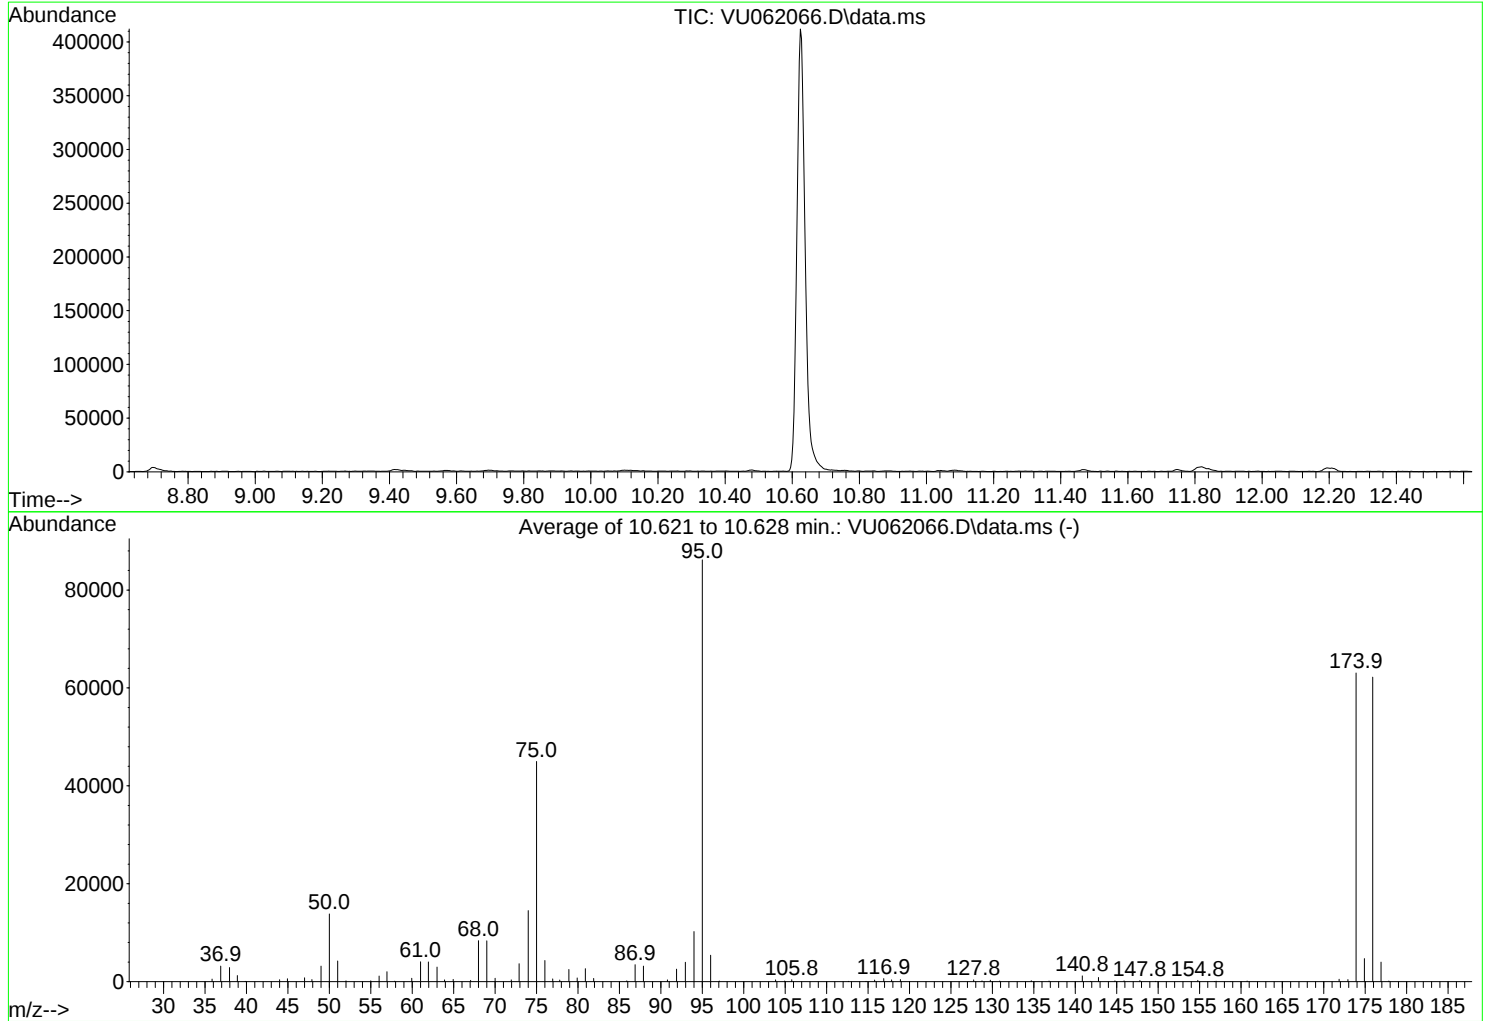

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2889

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.0	13816	PASS
75	95	30	80	52.2	44968	PASS
95	95	100	100	100.0	86171	PASS
96	95	5	9	6.3	5405	PASS
173	174	0.00	2	0.7	440	PASS
174	95	50	120	73.2	63051	PASS
175	174	5	9	7.5	4727	PASS
176	174	95	101	98.7	62205	PASS
177	176	5	9	6.4	3995	PASS

m/z	Abundance
35.90	397.0
37.80	146.0

Instrument :
MSVOA_U
ClientSampleId :
BFB039

m/z	Abundance
35.90	951.0
36.90	3244.0
38.00	2852.0
38.90	1235.0
44.00	394.0
45.00	547.0
47.00	745.0
47.90	426.0
49.00	3041.0
50.00	13550.0
51.00	4185.0
52.00	194.0
55.00	166.0
56.00	1182.0
56.90	2039.0
59.90	702.0
61.00	3822.0
61.90	3817.0
63.00	2851.0
63.90	353.0
65.00	481.0
67.10	321.0
68.00	7963.0
69.00	8054.0
70.00	694.0
71.90	364.0
72.90	3557.0
74.00	13990.0
75.00	43760.0
76.00	4215.0
77.00	612.0
77.80	339.0
78.90	2360.0
79.90	676.0
80.90	2511.0
81.90	597.0
85.90	141.0
86.90	3366.0
87.90	3033.0
90.80	302.0
91.90	2398.0
92.90	3813.0
94.00	9810.0
95.00	83576.0
96.00	5387.0
97.00	144.0
103.90	355.0
105.00	141.0
105.80	378.0
115.80	281.0
116.90	557.0
117.90	342.0
118.90	472.0
127.70	375.0
128.80	198.0
129.80	273.0
130.90	105.0
134.70	157.0
136.80	136.0
140.90	1113.0
141.90	115.0
142.80	849.0
144.70	129.0
145.90	151.0
147.80	182.0
149.70	120.0
154.80	226.0
156.80	123.0
160.80	104.0
171.80	474.0
173.90	59224.0
174.90	4462.0
175.90	58072.0
176.90	3986.0
177.90	135.0

Instrument :
MSVOA_U
ClientSampleId :
BFB039

m/z	Abundance
35.90	906.0
36.90	3280.0
38.00	3179.0
38.90	1273.0
39.80	106.0
44.00	407.0
44.90	613.0
47.00	819.0
47.90	453.0
49.00	3293.0
50.00	14237.0
51.00	4347.0
52.00	182.0
55.00	181.0
56.00	1190.0
56.90	2078.0
57.90	142.0
59.90	717.0
61.00	4161.0
62.00	4134.0
63.00	3093.0
63.90	373.0
65.00	483.0
67.00	267.0
68.00	8680.0
69.00	8596.0
70.00	718.0
71.90	337.0
72.90	3810.0
74.00	15130.0
75.00	46320.0
76.00	4505.0
76.90	589.0
77.80	346.0
78.90	2524.0
79.90	787.0
80.90	2739.0
81.90	674.0
85.90	172.0
86.90	3585.0
87.90	3243.0
90.80	395.0
91.90	2625.0
92.90	4048.0
94.00	10577.0
95.00	88928.0
96.00	5515.0
97.00	131.0
103.80	378.0
104.90	153.0
105.80	414.0
112.70	103.0
114.70	106.0
115.80	324.0
116.90	643.0
117.90	386.0
118.90	442.0
127.70	360.0
128.70	196.0
129.80	296.0
130.90	135.0
134.70	215.0
136.80	129.0
140.80	1212.0
141.80	109.0
142.80	883.0
144.80	161.0
145.90	163.0
147.80	238.0
149.70	113.0
154.80	274.0
157.00	140.0
160.70	129.0
171.90	513.0
172.90	662.0
173.90	64848.0
174.90	4903.0
175.90	64200.0
176.90	4154.0
177.90	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB039

m/z	Abundance
35.90	859.0
36.90	2960.0
38.00	3064.0
38.90	1223.0
39.90	118.0
44.00	433.0
44.90	600.0
47.00	795.0
47.90	440.0
49.00	3195.0
50.00	13660.0
51.00	4125.0
52.00	149.0
55.00	175.0
56.00	1106.0
57.00	1927.0
57.90	137.0
60.00	649.0
61.00	4216.0
62.00	4134.0
63.00	2944.0
63.90	366.0
64.90	423.0
67.00	247.0
68.00	8464.0
69.00	8342.0
70.00	639.0
72.00	343.0
72.90	3608.0
74.00	14456.0
75.00	44824.0
76.00	4238.0
76.90	495.0
77.80	355.0
78.90	2563.0
79.90	844.0
80.90	2683.0
81.90	659.0
85.90	149.0
86.90	3427.0
87.90	3268.0
90.80	426.0
91.90	2603.0
93.00	3982.0
94.00	10288.0
95.00	86008.0
96.00	5312.0
97.10	146.0
103.80	376.0
104.90	148.0
105.80	413.0
112.60	111.0
114.80	119.0
115.80	344.0
116.90	660.0
117.80	383.0
118.90	407.0
127.80	331.0
128.70	155.0
129.70	310.0
130.90	136.0
134.70	217.0
136.90	145.0
140.80	1191.0
142.80	870.0
144.90	170.0
145.90	144.0
147.80	258.0
154.80	280.0
157.00	122.0
158.80	120.0
160.70	131.0
171.80	515.0
172.90	658.0
173.90	65080.0
174.90	4817.0
175.90	64344.0
176.90	3846.0
177.80	122.0

Instrument :
MSVOA_U
ClientSampleId :
BFB039