

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120424\
 Data File : VU062086.D
 Acq On : 04 Dec 2024 10:16
 Operator : MD/SY
 Sample : VV1204WBL01
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Dec 05 01:30:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120324.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 05 01:30:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.257	114	16342	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.418	117	21503	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	7445	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	5509	0.477	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	96.000%
4) 1,2-Dichloroethane-d4	5.685	65	5960	0.499	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	100.000%
7) 1,2-Dichloropropane-d6	6.687	67	6547	0.535	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	106.000%
8) Toluene-d8	7.887	98	16668	0.507	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	102.000%
10) 1,1,2,2-Tetrachloroeth...	10.745	84	5337	0.519	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	104.000%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	13.110	75	119	0.079	ug/L	Qvalue # 74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120424\
Data File : VU062086.D
Acq On : 04 Dec 2024 10:16
Operator : MD/SY
Sample : VV1204WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Dec 05 01:30:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120324.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 05 01:30:27 2024
Response via : Initial Calibration

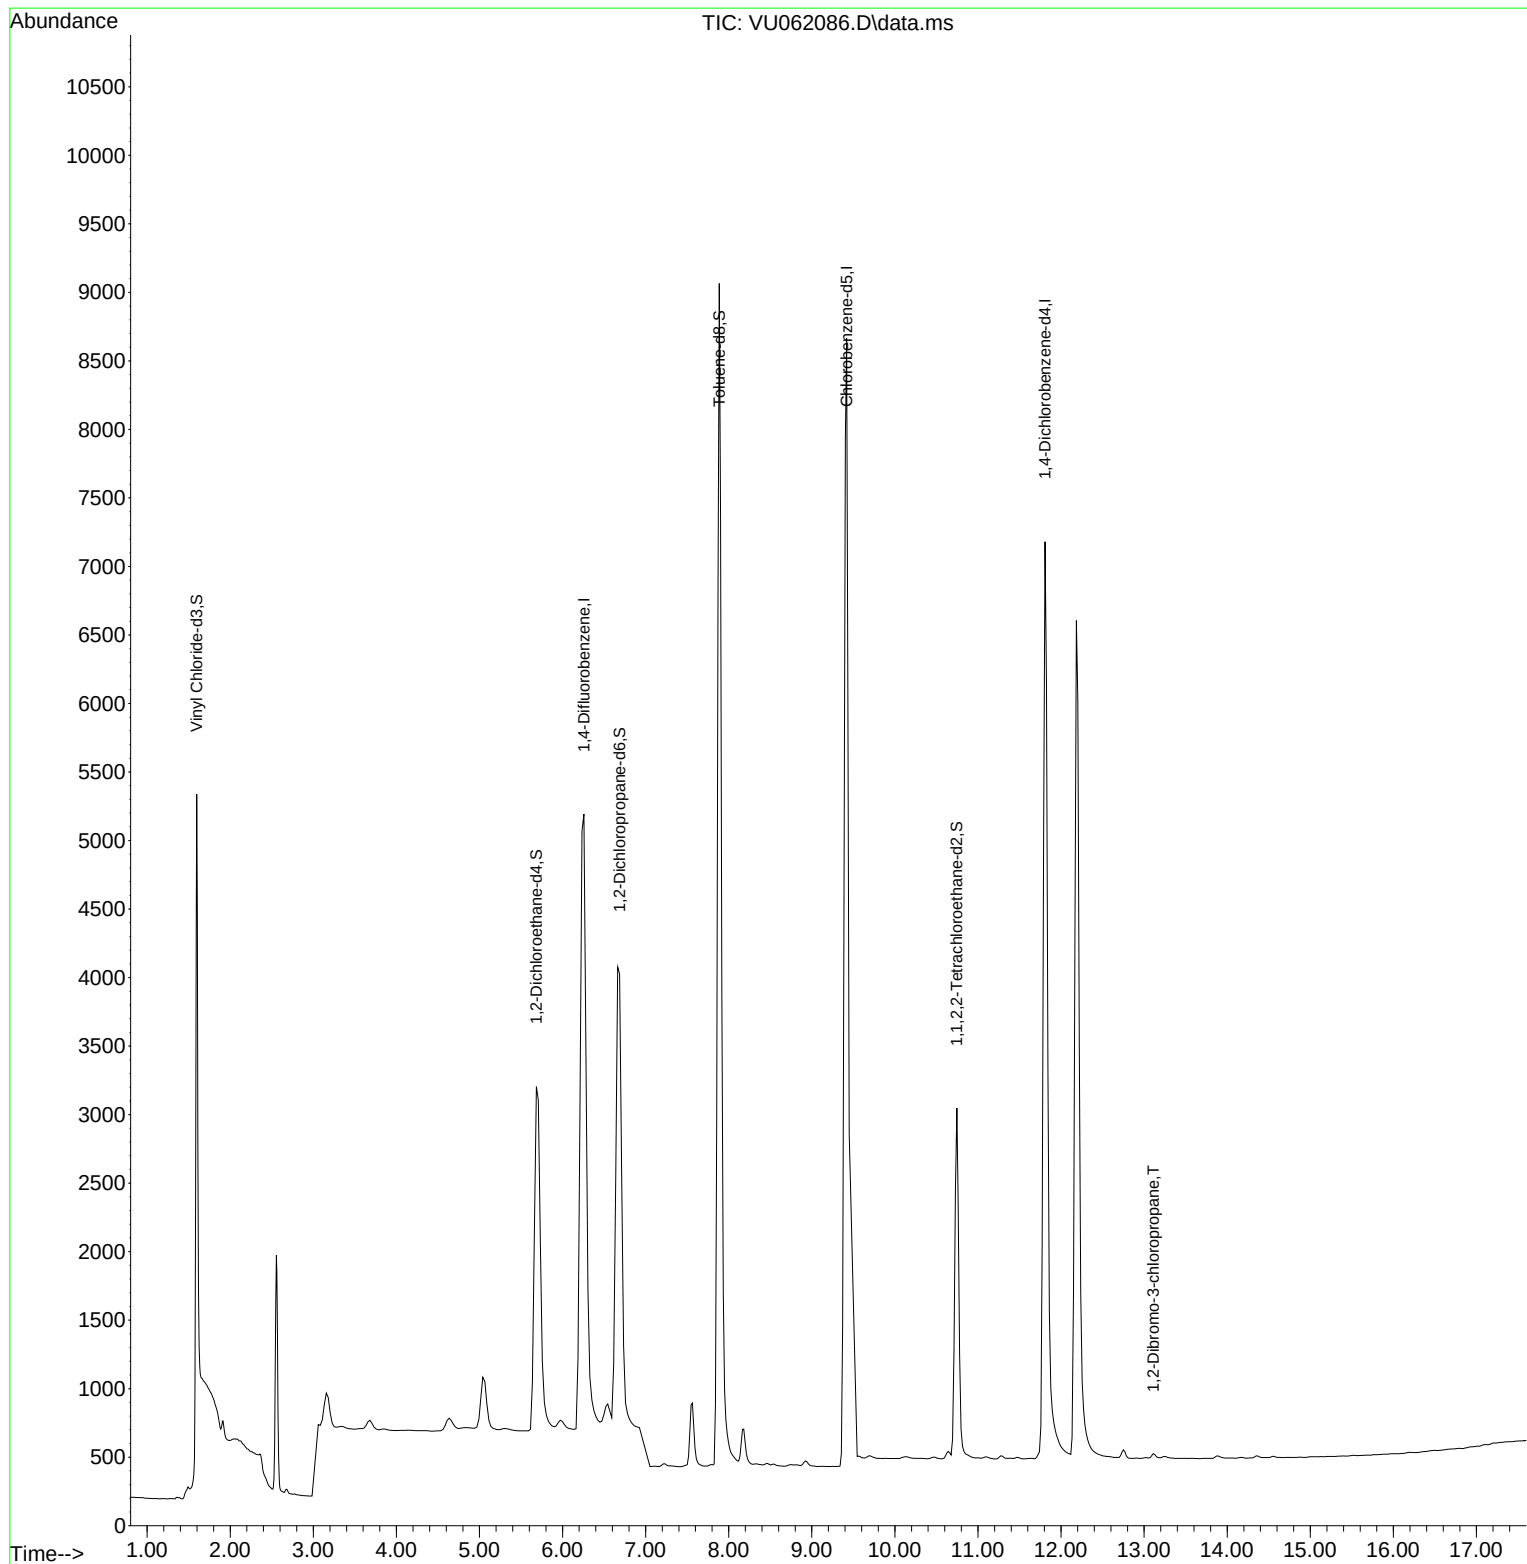

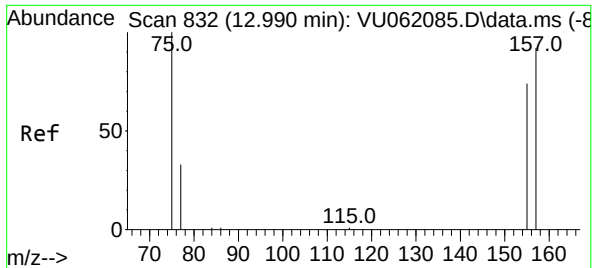

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.079 ug/L
 RT: 13.110 min Scan# 81
 Delta R.T. 0.120 min
 Lab File: VU062086.D
 Acq: 04 Dec 2024 10:16

Instrument :
 MSVOA_U
 ClientSampleId :

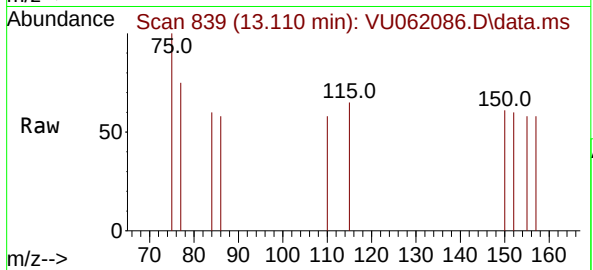

Tgt Ion: 75	Resp:	119
Ion Ratio	Lower	Upper
75	100	
157	57.5	69.4 104.2#
155	57.5	59.6 89.4#

