
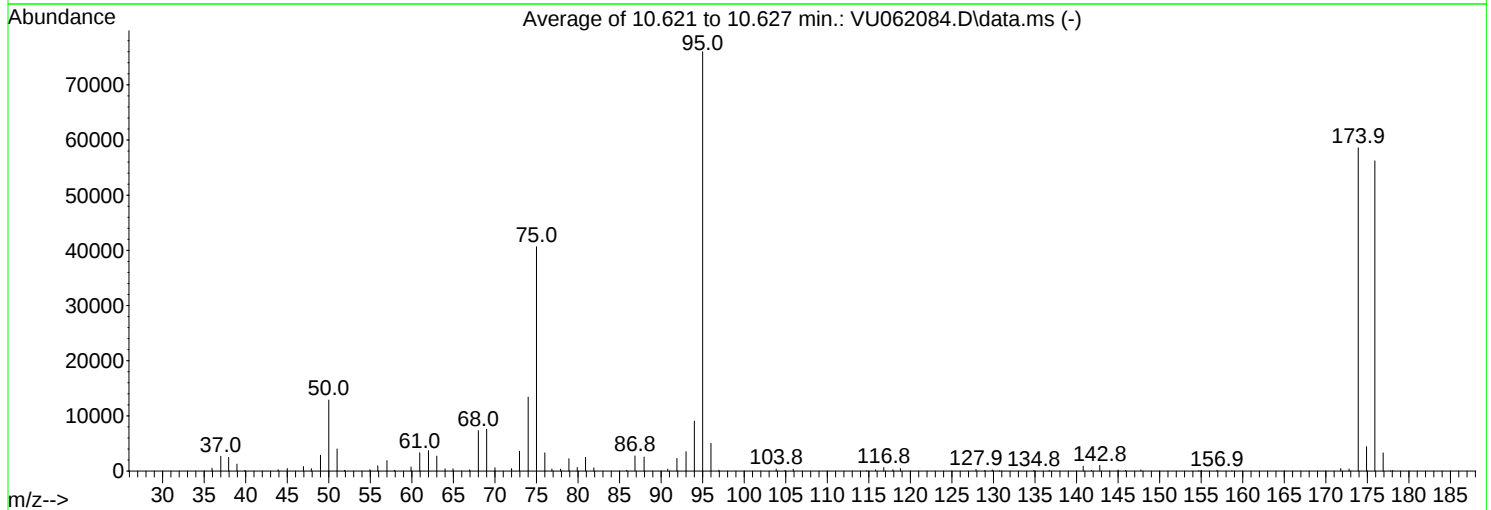


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120424\
Data File : VU062084.D
Acq On : 04 Dec 2024 08:16
Operator : MD/SY
Sample : BFB019
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB019

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120324.M
Title : TRACE VOA SOM01.0
Last Update : Thu Dec 05 01:30:27 2024

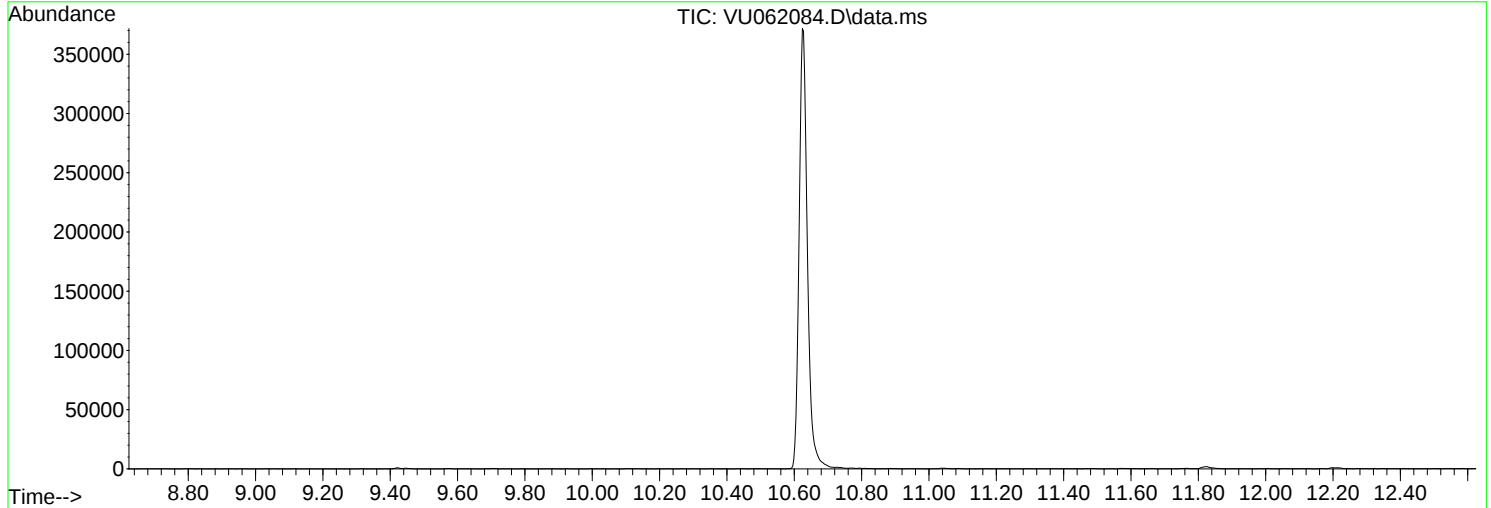

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	12877	PASS
75	95	30	80	53.5	40664	PASS
95	95	100	100	100.0	76005	PASS
96	95	5	9	6.6	5020	PASS
173	174	0.00	2	0.7	384	PASS
174	95	50	120	77.1	58592	PASS
175	174	5	9	7.5	4417	PASS
176	174	95	101	96.0	56237	PASS
177	176	5	9	5.9	3300	PASS

m/z	Abundance
43.90	175.0

Instrument :
MSVOA_U
ClientSampleId :
BFB019

m/z	Abundance
36.00	500.0
37.00	2651.0
38.00	2389.0
39.00	1100.0
39.90	101.0
43.90	467.0
45.00	495.0
46.90	795.0
47.90	457.0
49.00	2720.0
50.00	12372.0
51.00	3830.0
51.90	111.0
54.90	248.0
55.90	932.0
57.00	1746.0
57.90	117.0
59.90	764.0
60.90	3250.0
62.00	3448.0
63.00	2530.0
64.00	352.0
65.00	438.0
66.90	223.0
68.00	7056.0
69.00	7112.0
70.00	592.0
72.00	420.0
72.90	3500.0
74.00	12448.0
75.00	38440.0
76.00	3252.0
76.80	327.0
77.90	343.0
78.90	2185.0
79.90	593.0
80.90	2322.0
81.90	604.0
85.80	120.0
86.80	2571.0
87.90	2386.0
90.80	312.0
91.90	2170.0
93.00	3435.0
94.00	8468.0
95.00	71824.0
96.00	4817.0
96.90	151.0
103.80	385.0
104.90	135.0
105.90	318.0
115.80	246.0
116.80	653.0
117.90	237.0
118.80	443.0
127.90	292.0
128.90	112.0
129.90	216.0
134.90	129.0
136.70	156.0
140.80	791.0
141.80	131.0
142.80	975.0
145.00	188.0
145.90	115.0
147.70	195.0
154.70	195.0
156.90	144.0
171.80	401.0
172.80	578.0
173.90	54248.0
174.90	4167.0
175.90	51376.0
176.90	3173.0
177.80	136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB019

m/z	Abundance
35.90	541.0
37.00	2751.0
38.00	2530.0
38.90	1298.0
39.90	111.0
43.90	431.0
45.00	484.0
47.00	849.0
47.90	469.0
49.00	2958.0
50.00	13331.0
51.00	4100.0
51.90	130.0
55.00	268.0
55.90	984.0
57.00	1960.0
57.90	139.0
59.90	774.0
61.00	3458.0
62.00	3817.0
63.00	2791.0
64.00	445.0
65.00	421.0
66.90	233.0
68.00	7599.0
69.00	7857.0
70.00	644.0
72.00	505.0
73.00	3732.0
74.00	13928.0
75.00	41952.0
76.00	3424.0
76.90	400.0
77.90	356.0
78.90	2329.0
79.90	681.0
80.90	2597.0
81.90	613.0
85.80	134.0
86.90	2844.0
87.90	2581.0
90.80	375.0
91.90	2365.0
93.00	3631.0
94.00	9421.0
95.00	78368.0
96.00	5221.0
96.90	159.0
103.80	387.0
104.90	108.0
105.90	358.0
114.70	102.0
115.80	266.0
116.80	697.0
117.90	258.0
118.80	484.0
127.90	304.0
129.00	147.0
129.80	219.0
130.70	104.0
134.90	130.0
136.70	160.0
140.80	936.0
141.80	136.0
142.80	1086.0
145.00	206.0
145.90	111.0
147.80	215.0
155.00	219.0
156.90	165.0
171.80	496.0
172.80	573.0
173.90	60600.0
174.90	4581.0
175.90	58088.0
176.90	3400.0
178.00	118.0

Instrument :
MSVOA_U
ClientSampleId :
BFB019

m/z	Abundance
35.90	541.0
37.00	2662.0
37.90	2486.0
38.90	1388.0
39.90	102.0
43.90	419.0
45.00	466.0
47.00	811.0
47.90	418.0
49.00	2977.0
50.00	12927.0
51.00	4100.0
51.90	160.0
55.00	245.0
55.90	952.0
57.00	1991.0
57.90	145.0
59.90	712.0
61.00	3257.0
62.00	3846.0
63.00	2823.0
64.00	454.0
64.90	409.0
67.00	224.0
68.00	7328.0
69.00	7817.0
70.00	622.0
72.00	449.0
73.00	3573.0
74.00	13814.0
75.00	41600.0
76.00	3225.0
76.90	422.0
77.90	355.0
78.90	2238.0
79.90	701.0
80.90	2548.0
81.90	567.0
85.90	132.0
86.90	2850.0
88.00	2698.0
90.80	369.0
91.90	2352.0
93.00	3477.0
94.00	9297.0
95.00	77824.0
96.00	5023.0
97.00	158.0
103.90	357.0
105.90	337.0
114.80	118.0
115.80	278.0
116.80	606.0
117.90	281.0
118.80	473.0
127.90	305.0
129.00	160.0
129.80	233.0
130.80	124.0
134.80	123.0
136.70	138.0
140.80	949.0
141.80	121.0
142.80	1114.0
145.00	206.0
145.90	111.0
147.80	222.0
155.00	196.0
156.90	179.0
158.70	119.0
171.80	514.0
173.90	60928.0
174.90	4504.0
175.90	59248.0
176.90	3327.0
178.10	114.0

Instrument :
MSVOA_U
ClientSampleId :
BFB019