


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120524\
Data File : VU062089.D
Acq On : 05 Dec 2024 08:17
Operator : MD/SY
Sample : BFB081
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB081

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112724WMA.M
Title : VOC Analysis
Last Update : Fri Dec 06 00:44:17 2024

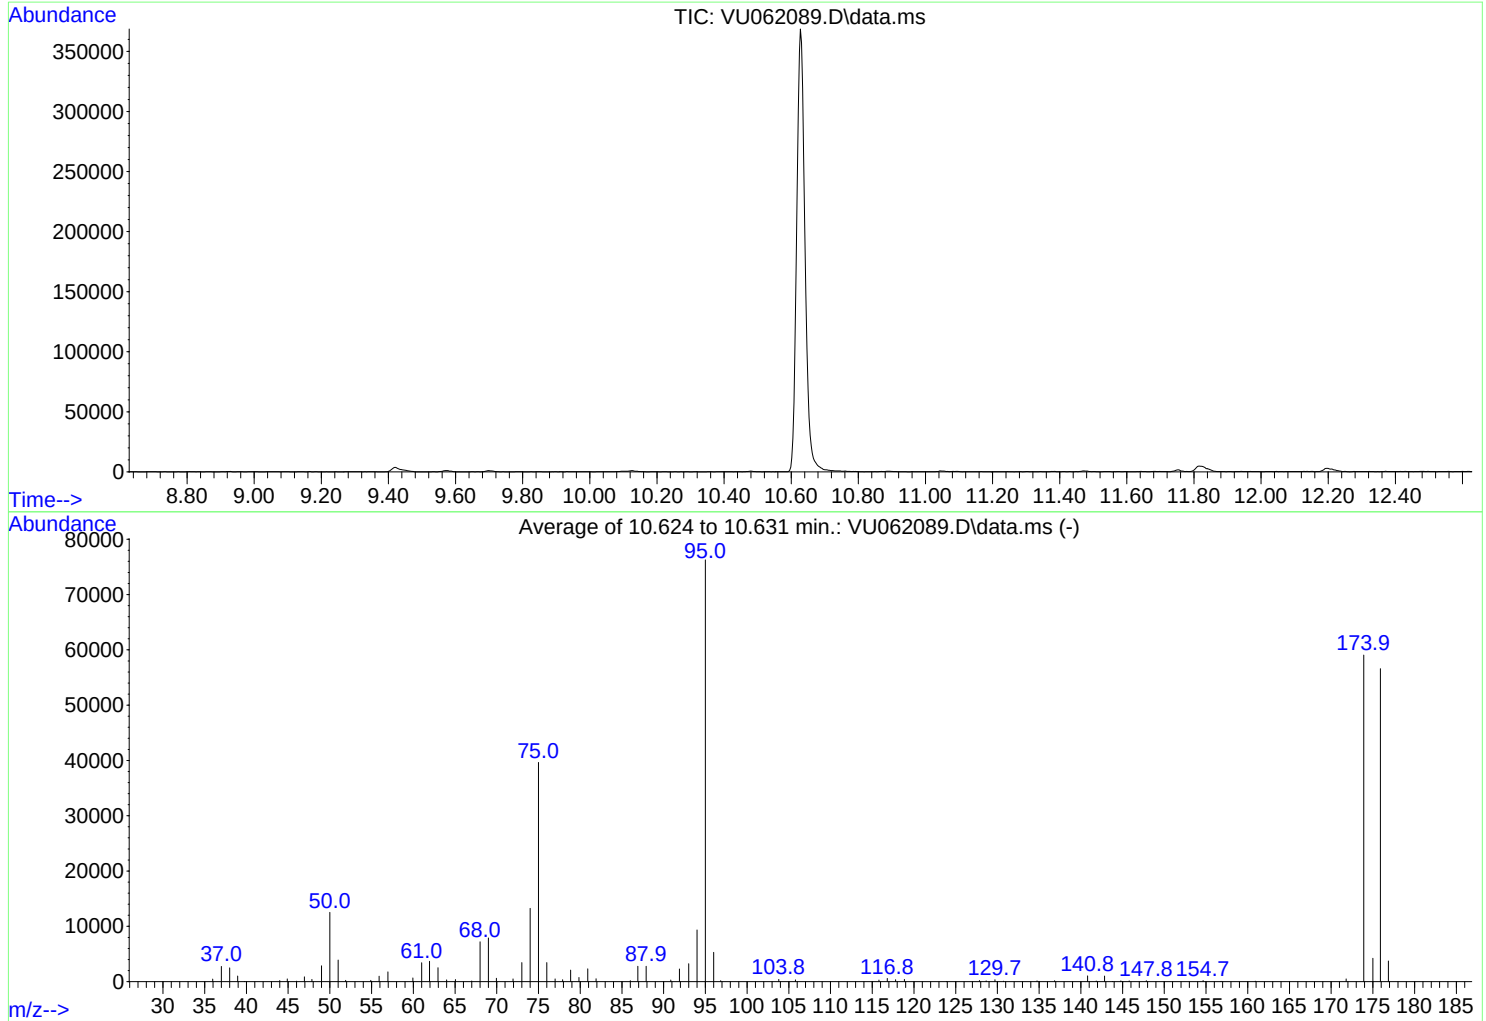

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	12518	PASS
75	95	30	80	52.0	39640	PASS
95	95	100	100	100.0	76280	PASS
96	95	5	9	6.9	5298	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.4	59045	PASS
175	174	5	9	7.1	4220	PASS
176	174	95	101	95.9	56595	PASS
177	176	5	9	6.6	3720	PASS

m/z	Abundance
44.00	172.0

Instrument :
MSVOA_U
ClientSampleId :
BFB081

m/z	Abundance
36.00	423.0
37.00	2669.0
38.00	2497.0
38.90	953.0
39.80	103.0
44.00	422.0
44.90	495.0
47.00	866.0
47.80	448.0
49.00	2828.0
50.00	12452.0
51.00	4020.0
51.90	213.0
54.90	241.0
55.90	992.0
57.00	1777.0
59.90	621.0
61.00	3422.0
62.00	3697.0
63.00	2589.0
64.00	324.0
65.10	382.0
67.10	188.0
68.00	6975.0
69.00	7612.0
69.90	599.0
72.00	507.0
73.00	3311.0
74.00	13224.0
75.00	38992.0
76.00	3474.0
77.00	552.0
77.90	315.0
78.90	2029.0
79.80	706.0
80.90	2390.0
81.90	462.0
86.00	182.0
86.90	2785.0
87.90	2696.0
90.90	327.0
91.90	2229.0
93.00	3225.0
94.00	9274.0
95.00	74840.0
96.00	5292.0
96.80	182.0
103.80	380.0
105.80	323.0
115.80	283.0
116.80	573.0
117.80	342.0
118.80	425.0
123.90	110.0
127.90	210.0
128.70	121.0
129.70	294.0
134.70	104.0
135.00	105.0
136.80	180.0
140.80	934.0
141.90	104.0
142.90	974.0
144.80	146.0
145.80	153.0
147.80	184.0
154.60	174.0
156.80	110.0
160.90	151.0
171.70	385.0
173.90	56480.0
175.00	4097.0
175.90	53584.0
176.80	3622.0

Instrument :
MSVOA_U
ClientSampleId :
BFB081

m/z	Abundance
35.90	476.0
37.00	2795.0
38.00	2548.0
38.90	1033.0
44.00	390.0
44.90	504.0
46.00	135.0
46.90	909.0
47.90	402.0
49.00	2927.0
50.00	12838.0
51.00	4005.0
51.90	222.0
54.90	242.0
55.90	1015.0
56.90	1808.0
60.00	677.0
61.00	3496.0
61.90	3801.0
63.00	2561.0
64.00	315.0
65.10	362.0
68.00	7417.0
69.00	8225.0
69.90	636.0
72.00	499.0
73.00	3512.0
74.00	13625.0
75.00	40600.0
76.00	3514.0
77.00	522.0
77.90	376.0
78.80	2115.0
79.90	796.0
80.90	2355.0
81.90	522.0
86.00	177.0
86.90	2878.0
87.90	2934.0
90.90	308.0
91.90	2366.0
93.00	3313.0
94.00	9639.0
95.00	78600.0
96.00	5473.0
96.80	196.0
103.80	428.0
105.80	330.0
115.80	294.0
116.80	595.0
117.80	361.0
118.90	426.0
127.80	217.0
128.60	145.0
129.70	361.0
130.80	119.0
134.70	139.0
136.80	174.0
140.80	1078.0
141.90	138.0
142.90	1046.0
144.80	145.0
145.80	175.0
147.90	183.0
154.70	227.0
156.80	108.0
160.90	148.0
171.80	492.0
173.90	60712.0
175.00	4384.0
175.90	58288.0
176.90	3858.0

Instrument :
MSVOA_U
ClientSampleId :
BFB081

m/z	Abundance
35.90	483.0
37.00	2833.0
38.00	2440.0
39.00	1035.0
44.00	338.0
44.90	471.0
46.00	112.0
46.90	794.0
47.90	348.0
49.00	2805.0
50.00	12265.0
51.00	3668.0
51.90	225.0
54.90	215.0
55.90	946.0
56.90	1760.0
59.90	684.0
61.00	3330.0
61.90	3571.0
62.90	2428.0
64.00	309.0
64.90	370.0
66.90	167.0
68.00	7197.0
69.00	7890.0
70.00	612.0
71.90	476.0
73.00	3501.0
74.00	12883.0
75.00	39328.0
76.00	3386.0
77.00	414.0
77.90	370.0
78.80	2131.0
79.90	782.0
80.90	2166.0
81.90	548.0
86.00	133.0
86.90	2663.0
87.90	2728.0
90.80	285.0
91.90	2298.0
93.00	3171.0
94.00	9117.0
95.00	75400.0
96.00	5129.0
96.90	175.0
103.80	434.0
105.80	348.0
115.80	279.0
116.80	550.0
117.80	322.0
118.90	402.0
127.90	208.0
128.60	145.0
129.70	358.0
130.70	138.0
134.80	168.0
136.90	138.0
140.80	1088.0
141.80	137.0
142.80	1001.0
143.80	104.0
144.80	160.0
145.80	147.0
147.80	183.0
154.70	250.0
171.90	583.0
173.90	59944.0
175.00	4178.0
175.90	57912.0
176.90	3679.0

Instrument :
MSVOA_U
ClientSampleId :
BFB081