


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120624\
Data File : VU062096.D
Acq On : 05 Dec 2024 13:27
Operator : MD/SY
Sample : BFB040
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB040

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR112024WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Dec 06 02:27:00 2024

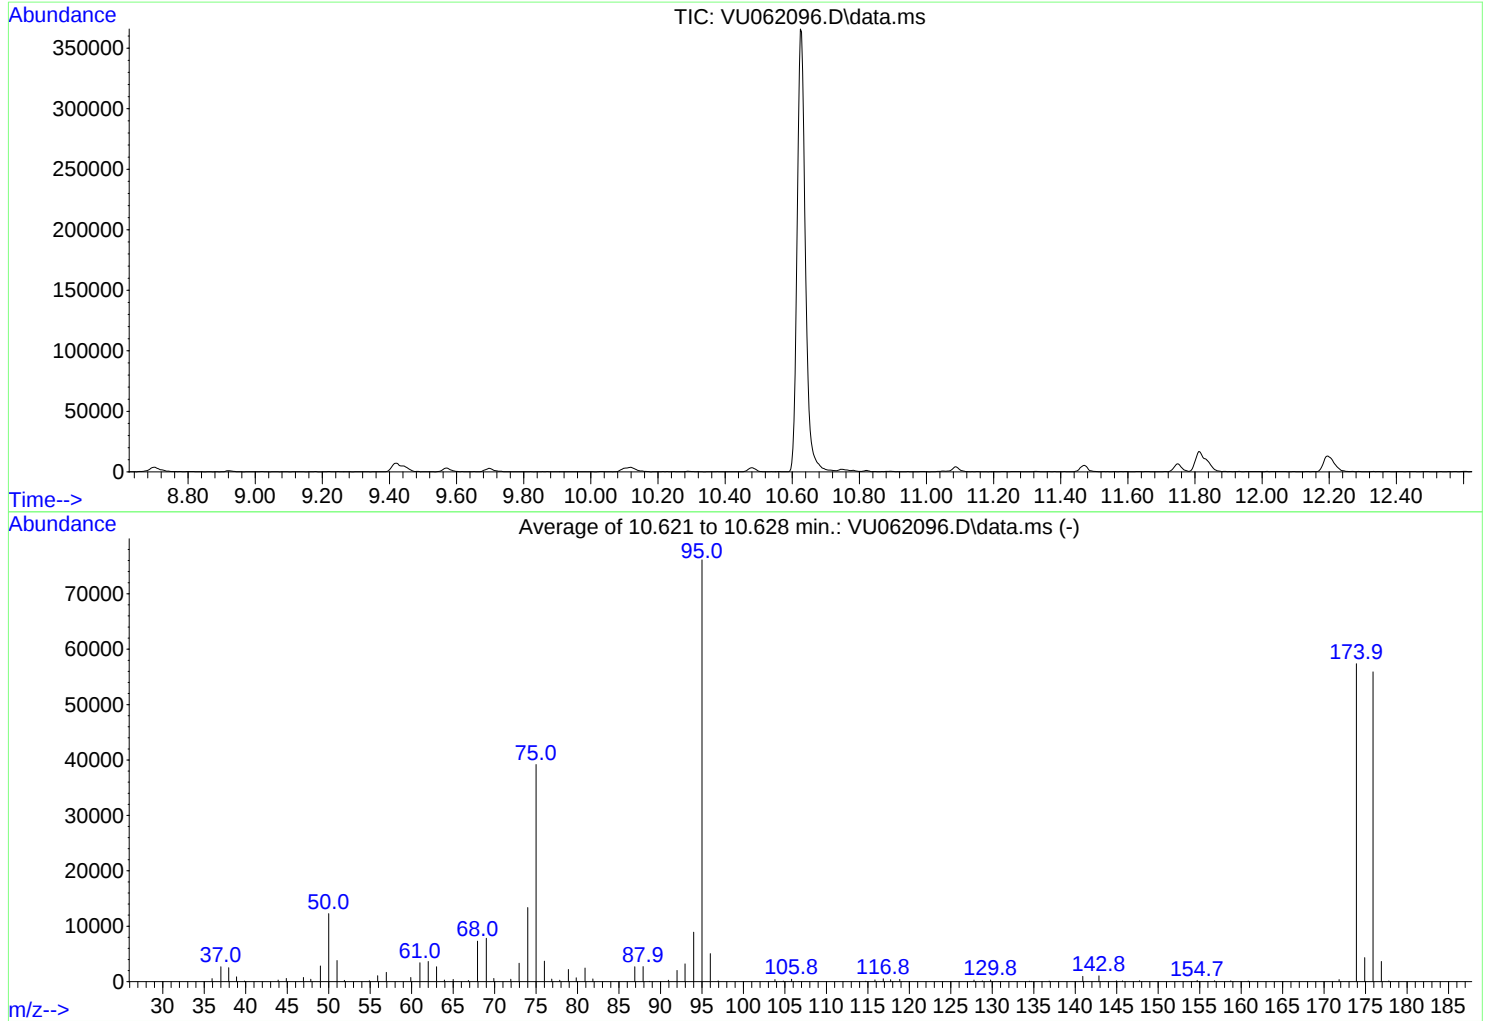

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.1	12281	PASS
75	95	30	80	51.5	39181	PASS
95	95	100	100	100.0	76128	PASS
96	95	5	9	6.6	5062	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.4	57368	PASS
175	174	5	9	7.5	4326	PASS
176	174	95	101	97.4	55901	PASS
177	176	5	9	6.5	3647	PASS

m/z	Abundance
43.90	187.0

Instrument :
MSVOA_U
ClientSampleId :
BFB040

m/z	Abundance
36.00	539.0
37.00	2588.0
38.00	2448.0
38.90	881.0
39.90	113.0
43.90	401.0
44.90	562.0
46.90	742.0
47.80	393.0
49.00	2752.0
50.00	11879.0
51.00	3740.0
51.90	251.0
54.90	161.0
55.90	1028.0
56.90	1645.0
59.90	748.0
61.00	3391.0
62.00	3672.0
63.00	2642.0
64.00	255.0
65.00	394.0
66.80	185.0
68.00	6856.0
69.00	7355.0
69.90	584.0
72.00	450.0
72.90	3208.0
74.00	12921.0
75.00	36856.0
76.00	3514.0
76.90	423.0
77.90	263.0
78.90	2145.0
79.80	652.0
80.90	2385.0
81.90	462.0
86.90	2608.0
87.90	2522.0
91.00	272.0
92.00	2012.0
92.90	3010.0
94.00	8459.0
95.00	72144.0
96.00	4902.0
96.90	145.0
103.80	314.0
104.80	134.0
105.80	422.0
115.80	289.0
116.90	528.0
117.80	307.0
118.80	373.0
127.80	241.0
128.80	144.0
129.80	297.0
134.50	107.0
136.80	116.0
140.90	913.0
142.80	936.0
144.90	151.0
145.60	129.0
147.80	147.0
154.70	225.0
156.80	164.0
158.70	148.0
160.80	124.0
171.80	382.0
173.90	53352.0
174.90	4133.0
175.90	51192.0
176.90	3431.0
177.80	145.0

Instrument :
MSVOA_U
ClientSampleId :
BFB040

m/z	Abundance
36.00	573.0
37.00	2792.0
38.00	2642.0
38.90	887.0
39.80	107.0
43.90	479.0
44.90	598.0
47.00	777.0
47.80	431.0
49.00	2969.0
50.00	12665.0
51.00	3897.0
51.90	239.0
54.90	158.0
55.90	1114.0
56.90	1712.0
59.90	798.0
61.00	3484.0
62.00	3732.0
63.00	2769.0
63.90	276.0
65.00	422.0
66.90	217.0
67.90	7524.0
69.00	8133.0
69.90	597.0
72.00	430.0
72.90	3366.0
74.00	13844.0
75.00	40496.0
76.00	3912.0
76.90	470.0
77.80	262.0
78.90	2273.0
79.80	706.0
80.90	2484.0
81.90	505.0
86.90	2833.0
87.90	2778.0
90.90	275.0
92.00	2129.0
92.90	3253.0
94.00	9209.0
95.00	78464.0
96.00	5206.0
97.00	148.0
103.80	378.0
104.80	132.0
105.80	447.0
114.80	106.0
115.90	334.0
116.90	533.0
117.70	348.0
118.90	429.0
127.80	308.0
128.80	149.0
129.80	313.0
130.80	102.0
134.50	129.0
136.90	128.0
140.90	998.0
142.80	1072.0
145.00	153.0
145.70	150.0
147.70	167.0
154.70	239.0
156.80	179.0
158.70	154.0
160.90	116.0
171.80	386.0
173.90	59048.0
174.90	4405.0
175.90	57944.0
176.90	3754.0
177.80	176.0

Instrument :
MSVOA_U
ClientSampleId :
BFB040

m/z	Abundance
35.90	546.0
37.00	2727.0
37.90	2458.0
38.90	848.0
39.80	107.0
43.90	532.0
44.90	591.0
47.00	712.0
47.90	449.0
49.00	2751.0
50.00	12300.0
51.00	3788.0
51.90	198.0
54.90	171.0
55.90	1099.0
57.00	1702.0
59.90	740.0
61.00	3342.0
62.00	3484.0
63.00	2639.0
63.90	316.0
65.00	422.0
66.90	212.0
67.90	7514.0
69.00	7995.0
69.90	530.0
71.90	443.0
73.00	3431.0
74.00	13368.0
75.00	40192.0
76.00	3688.0
76.90	468.0
77.90	255.0
78.90	2211.0
79.90	774.0
80.90	2480.0
81.80	547.0
86.90	2663.0
87.90	2850.0
88.70	182.0
90.90	247.0
92.00	1965.0
93.00	3332.0
94.00	9091.0
95.00	77776.0
96.00	5077.0
96.90	142.0
103.80	438.0
104.80	119.0
105.80	422.0
106.70	105.0
114.70	125.0
115.90	343.0
116.80	522.0
117.70	360.0
118.90	436.0
127.80	317.0
128.80	165.0
129.80	307.0
134.70	154.0
136.80	122.0
140.90	1001.0
142.90	1098.0
145.00	139.0
145.80	169.0
147.70	177.0
154.70	214.0
156.80	165.0
158.80	132.0
160.80	106.0
171.80	386.0
173.90	59704.0
174.90	4440.0
175.90	58568.0
176.90	3755.0
177.80	141.0

Instrument :
MSVOA_U
ClientSampleId :
BFB040