

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120724\
 Data File : VU062131.D
 Acq On : 06 Dec 2024 14:06
 Operator : MD/SY
 Sample : P5109-02
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHJA1

Quant Time: Dec 06 23:15:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR112024WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Dec 06 02:27:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	106187	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	97180	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	45379	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	18439	3.540	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	70.800%
7) Chloroethane-d5	1.911	69	16393	3.558	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	71.200%
11) 1,1-Dichloroethene-d2	2.560	65	8446	4.059	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.200%
20) 2-Butanone-d5	4.627	46	63514	38.831	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	77.660%
24) Chloroform-d	5.049	84	57166	4.499	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.000%
26) 1,2-Dichloroethane-d4	5.692	65	30332	4.638	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.800%
32) Benzene-d6	5.717	84	93076	4.916	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.400%
36) 1,2-Dichloropropane-d6	6.679	67	32063	4.984	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.600%
41) Toluene-d8	7.891	98	76906	4.870	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.400%
43) trans-1,3-Dichloroprop...	8.171	79	12296	5.163	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	103.200%
46) 2-Hexanone-d5	8.627	63	44063	40.532	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.060%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	27147	4.223	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.400%
66) 1,2-Dichlorobenzene-d4	12.183	152	33982	5.064	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.200%
Target Compounds						
22) cis-1,2-Dichloroethene	4.660	96	13367	1.578	ug/L	91
34) Trichloroethene	6.531	95	39624	5.059	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120724\
Data File : VU062131.D
Acq On : 06 Dec 2024 14:06
Operator : MD/SY
Sample : P5109-02
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHJA1

Quant Time: Dec 06 23:15:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR112024WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Dec 06 02:27:00 2024
Response via : Initial Calibration




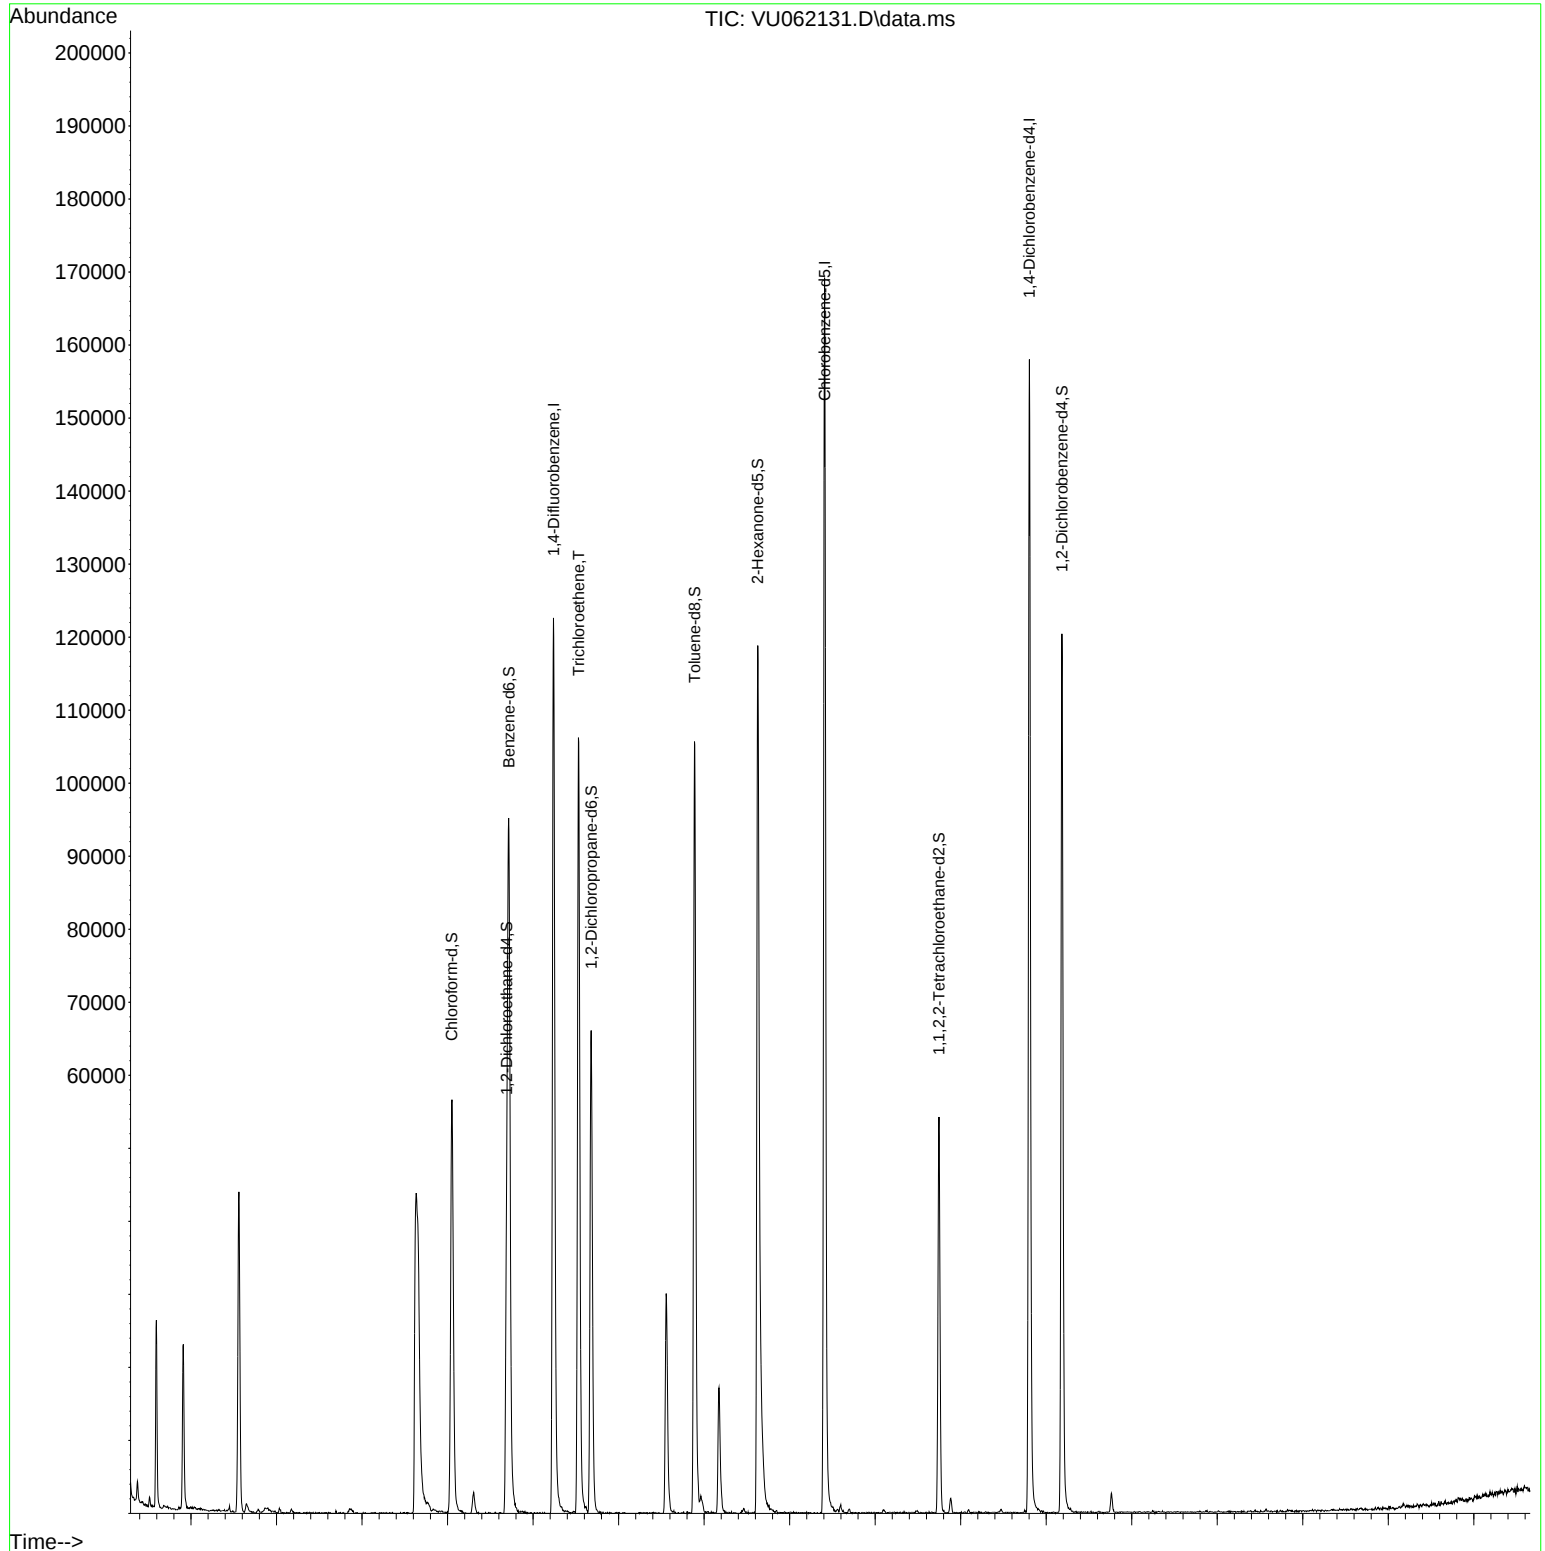


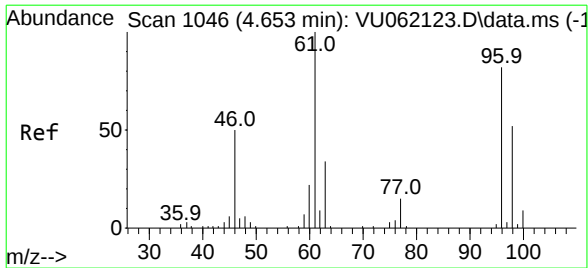

#22
 cis-1,2-Dichloroethene
 Concen: 1.578 ug/L
 RT: 4.660 min Scan# 1046
 Delta R.T. 0.003 min
 Lab File: VU062131.D
 Acq: 06 Dec 2024 14:06

Instrument :
 MSVOA_U
 ClientSampleId :
 BHJA1

Tgt Ion: 96	Resp: 13367
Ion Ratio	Lower Upper
96 100	
61 116.5	92.0 170.8
98 62.4	44.5 82.7

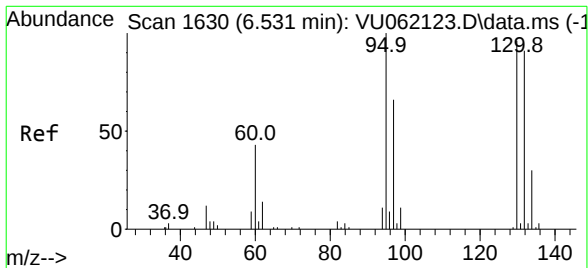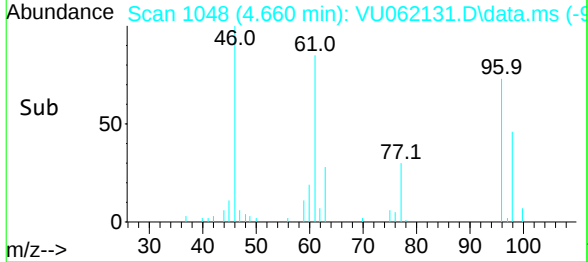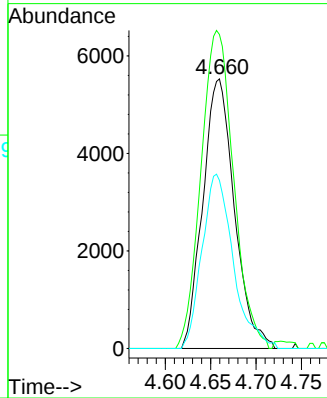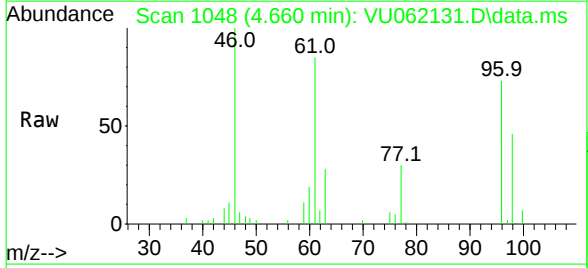

#34
 Trichloroethene
 Concen: 5.059 ug/L
 RT: 6.531 min Scan# 1630
 Delta R.T. -0.003 min
 Lab File: VU062131.D
 Acq: 06 Dec 2024 14:06

Tgt Ion: 95	Resp: 39624
Ion Ratio	Lower Upper
95 100	
97 63.3	45.9 85.3
132 89.0	63.8 118.4
130 96.2	65.5 121.7

