
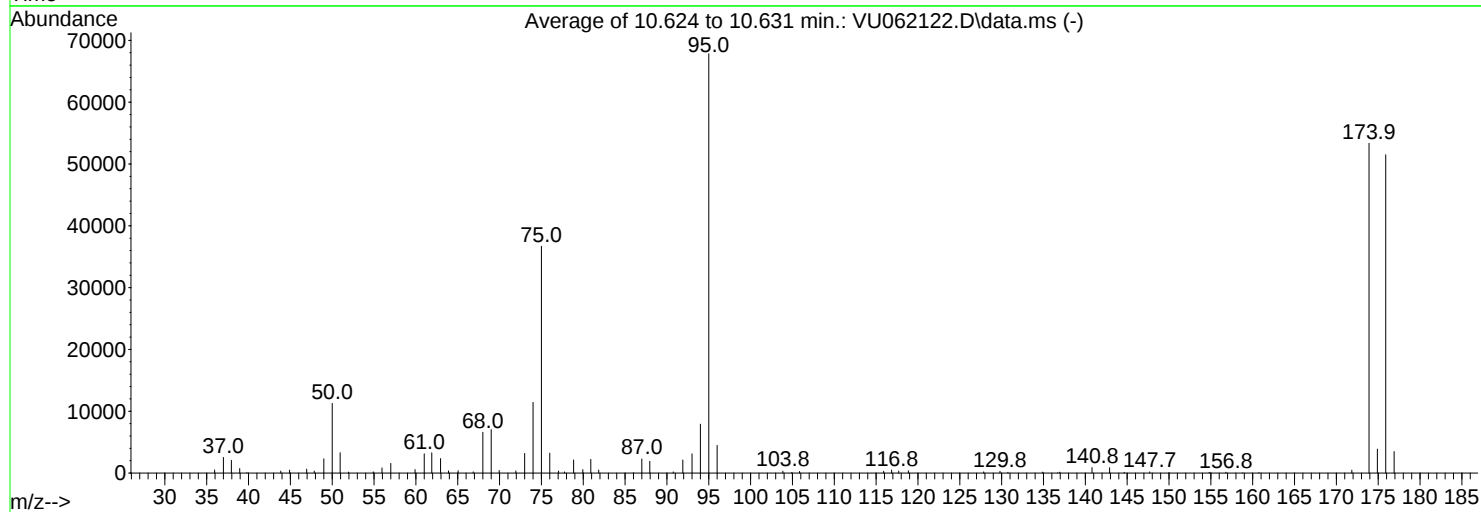


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120724\
Data File : VU062122.D
Acq On : 06 Dec 2024 09:11
Operator : MD/SY
Sample : BFB041
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB041

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR112024WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Dec 06 02:27:00 2024

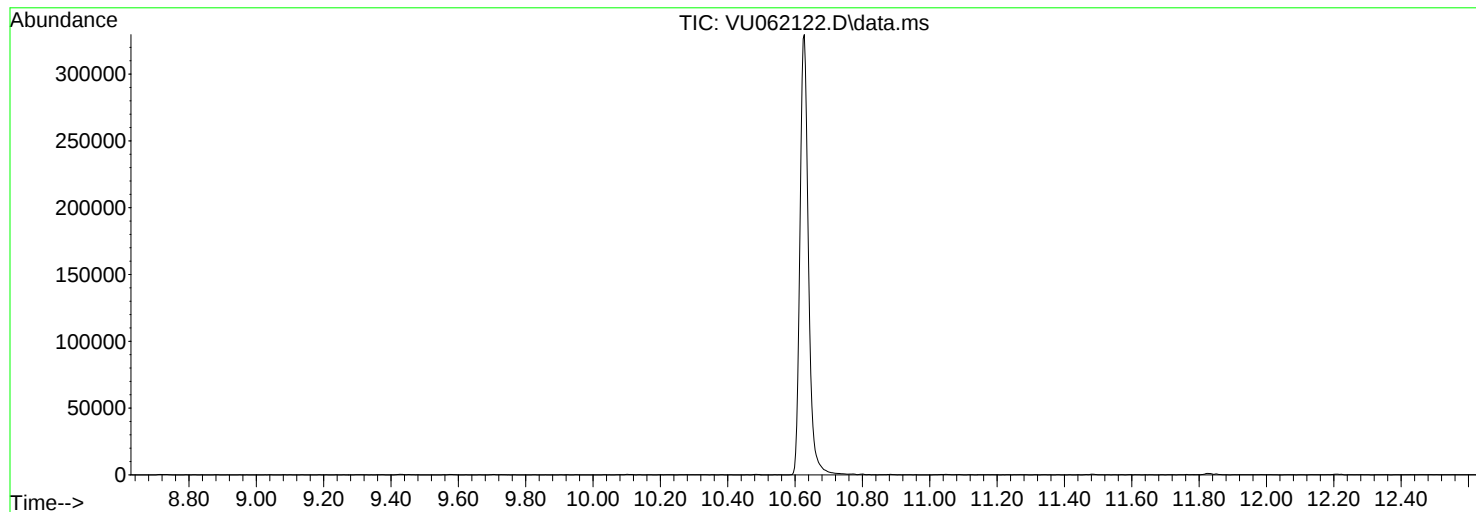

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	11274	PASS
75	95	30	80	54.1	36691	PASS
95	95	100	100	100.0	67840	PASS
96	95	5	9	6.6	4481	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.7	53357	PASS
175	174	5	9	7.3	3886	PASS
176	174	95	101	96.5	51501	PASS
177	176	5	9	6.8	3486	PASS

m/z

Abundance

Instrument :

MSVOA_U

ClientSampleId :

BFB041

m/z	Abundance
35.90	515.0
37.00	2429.0
38.00	2093.0
38.90	729.0
43.90	314.0
44.90	507.0
46.90	631.0
47.90	308.0
49.00	2486.0
50.00	11761.0
51.00	3526.0
52.00	174.0
54.90	190.0
56.00	877.0
57.00	1675.0
59.90	562.0
61.00	3083.0
61.90	3318.0
62.90	2464.0
63.90	330.0
65.00	459.0
66.90	224.0
68.00	6901.0
69.00	7464.0
70.00	460.0
71.90	358.0
73.00	3248.0
74.00	11688.0
75.00	37456.0
76.00	3306.0
77.00	350.0
77.90	172.0
78.90	2131.0
79.90	659.0
80.90	2287.0
81.90	480.0
86.00	101.0
87.00	2244.0
87.90	2001.0
90.80	206.0
91.90	2230.0
93.00	3131.0
94.00	8141.0
95.00	69224.0
96.00	4567.0
103.80	320.0
105.90	297.0
115.90	293.0
116.80	496.0
117.70	375.0
118.80	403.0
127.80	235.0
129.80	316.0
130.80	140.0
134.90	160.0
136.90	167.0
140.80	935.0
142.90	904.0
144.70	128.0
147.70	170.0
150.00	109.0
154.80	192.0
156.80	147.0
171.90	445.0
173.90	53416.0
174.90	4206.0
175.90	51584.0
176.90	3491.0

Instrument :
MSVOA_U
ClientSampleId :
BFB041

m/z	Abundance
36.00	531.0
37.00	2585.0
37.90	2109.0
38.90	737.0
39.80	107.0
43.80	329.0
44.90	522.0
47.00	655.0
47.90	340.0
49.00	2346.0
50.00	11556.0
51.00	3321.0
51.90	164.0
54.90	214.0
56.00	872.0
57.00	1574.0
59.90	564.0
61.00	3167.0
61.90	3332.0
63.00	2392.0
63.90	370.0
65.10	395.0
66.80	213.0
68.00	6813.0
69.00	7244.0
70.00	437.0
72.00	348.0
73.00	3305.0
74.00	11707.0
75.00	37904.0
76.00	3295.0
77.00	339.0
77.70	205.0
78.90	2169.0
79.90	565.0
80.90	2267.0
81.80	515.0
87.00	2306.0
88.00	1925.0
90.70	194.0
91.90	2152.0
93.00	3210.0
94.00	8036.0
95.00	69624.0
96.00	4622.0
103.90	320.0
104.90	106.0
105.90	278.0
115.90	299.0
116.90	501.0
117.70	335.0
118.80	383.0
127.80	205.0
129.80	307.0
130.80	134.0
134.90	179.0
137.00	152.0
140.80	910.0
142.90	888.0
144.70	131.0
147.70	203.0
150.00	101.0
154.80	157.0
156.80	150.0
160.80	107.0
171.80	511.0
173.90	55000.0
174.90	3971.0
175.90	53024.0
176.90	3603.0

Instrument :
MSVOA_U
ClientSampleId :
BFB041

m/z	Abundance
35.90	476.0
37.00	2583.0
37.90	1979.0
39.00	745.0
39.80	117.0
43.80	334.0
44.90	434.0
47.00	622.0
47.80	355.0
49.00	2103.0
50.00	10506.0
50.90	3058.0
51.90	148.0
54.90	228.0
55.90	789.0
57.00	1473.0
59.90	588.0
61.00	3085.0
61.90	3159.0
63.00	2186.0
63.90	345.0
65.00	301.0
66.90	165.0
68.00	6082.0
69.00	6431.0
69.90	381.0
71.90	357.0
73.00	3008.0
74.00	10953.0
75.00	34712.0
76.00	3099.0
77.10	308.0
77.70	209.0
78.80	2075.0
80.00	481.0
80.90	2081.0
81.80	513.0
87.00	2303.0
87.90	1772.0
90.80	186.0
91.90	1987.0
93.00	3023.0
94.00	7562.0
95.00	64672.0
96.00	4254.0
103.90	348.0
104.90	107.0
105.80	235.0
115.90	305.0
116.90	474.0
117.70	291.0
118.90	359.0
127.90	176.0
129.80	262.0
130.70	131.0
134.90	149.0
136.70	109.0
137.00	140.0
140.80	820.0
142.90	834.0
144.60	135.0
147.70	204.0
155.00	123.0
156.80	124.0
158.80	102.0
160.70	106.0
171.80	469.0
173.90	51656.0
174.90	3481.0
175.90	49896.0
176.90	3364.0

Instrument :
MSVOA_U
ClientSampleId :
BFB041