


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121024\
Data File : VU062204.D
Acq On : 10 Dec 2024 13:04
Operator : MD/SY
Sample : BFB043
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB043

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Dec 11 03:43:25 2024

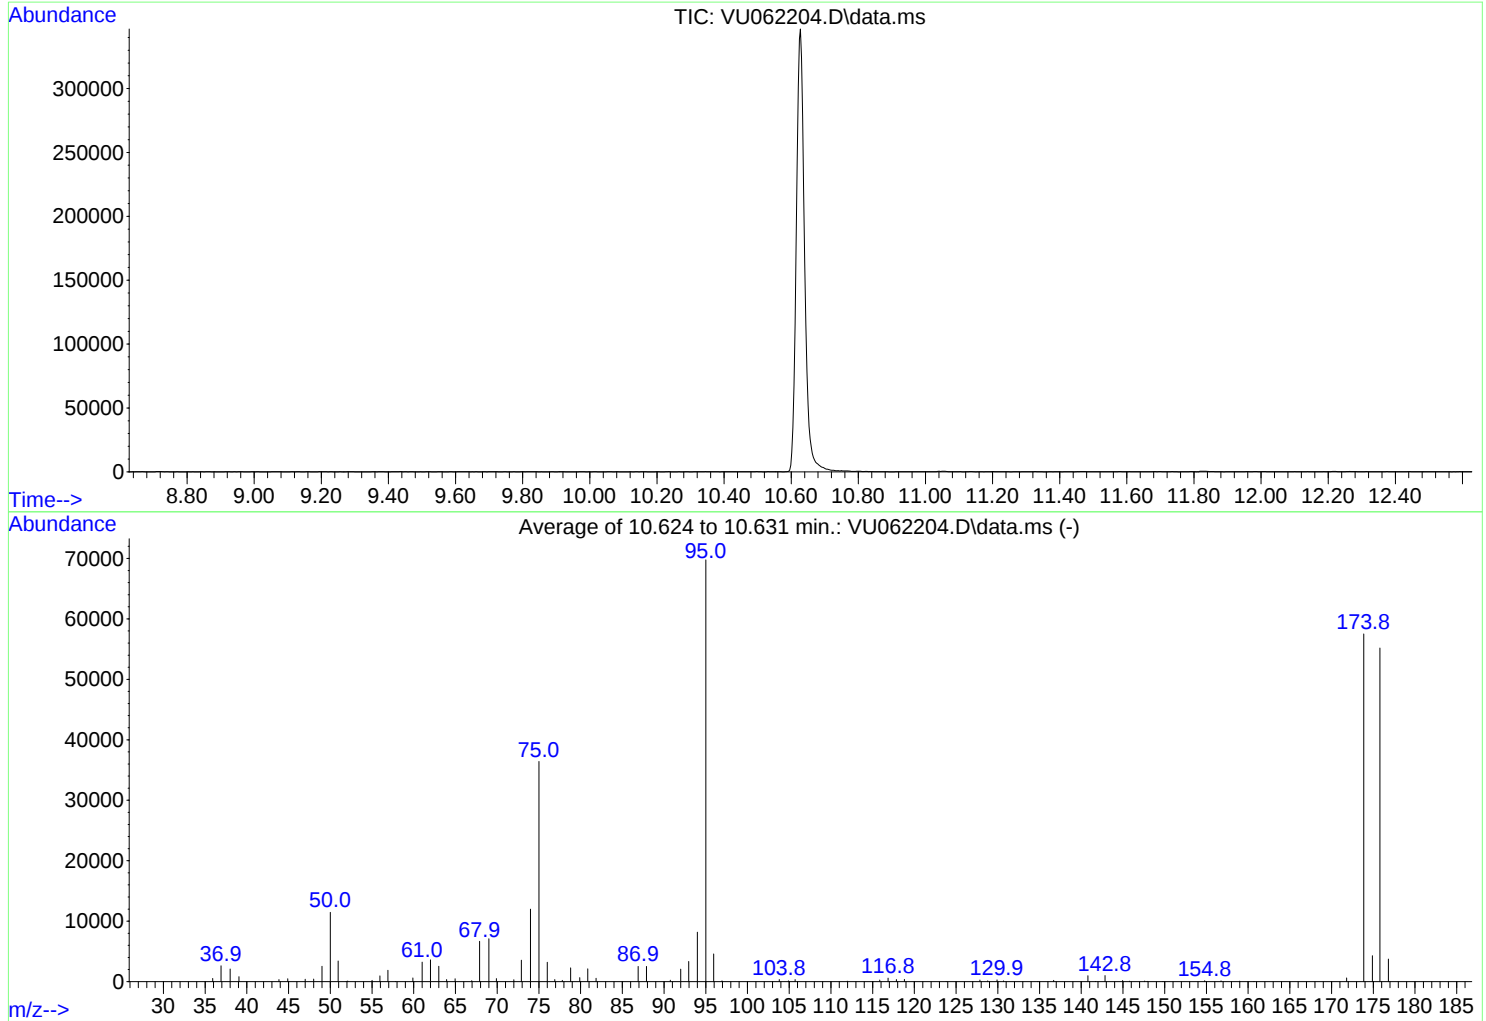

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	11475	PASS
75	95	30	80	52.2	36429	PASS
95	95	100	100	100.0	69768	PASS
96	95	5	9	6.6	4595	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.4	57520	PASS
175	174	5	9	7.5	4300	PASS
176	174	95	101	95.9	55179	PASS
177	176	5	9	6.8	3746	PASS

m/z	Abundance
43.80	110.0

Instrument :
MSVOA_U
ClientSampleId :
BFB043

m/z	Abundance
35.90	597.0
36.90	2749.0
38.00	2037.0
39.00	808.0
43.90	508.0
44.90	468.0
47.00	409.0
48.00	427.0
49.00	2598.0
50.00	11704.0
50.90	3657.0
51.90	139.0
55.00	205.0
56.00	953.0
56.90	1812.0
59.90	632.0
61.00	3312.0
62.00	3684.0
63.00	2612.0
63.90	392.0
64.90	509.0
66.90	185.0
67.90	6651.0
69.00	7018.0
69.90	463.0
72.00	309.0
72.90	3569.0
74.00	12355.0
75.00	37024.0
76.00	3432.0
76.90	318.0
77.80	270.0
78.80	2276.0
79.90	675.0
80.90	2215.0
81.80	551.0
86.90	2518.0
87.90	2567.0
90.70	262.0
92.00	2036.0
92.90	3396.0
94.00	8357.0
95.00	70184.0
95.90	4630.0
96.90	155.0
103.80	358.0
104.90	133.0
105.70	319.0
115.90	295.0
116.80	612.0
117.80	348.0
118.90	390.0
127.80	293.0
128.80	114.0
129.90	264.0
130.70	125.0
136.70	234.0
140.80	947.0
141.70	115.0
142.90	1055.0
145.00	203.0
145.80	119.0
147.60	165.0
154.80	174.0
156.80	131.0
160.70	104.0
171.80	606.0
173.80	57072.0
174.90	4316.0
175.80	54952.0
176.80	3760.0

Instrument :
MSVOA_U
ClientSampleId :
BFB043

m/z	Abundance
35.90	555.0
36.90	2741.0
38.00	2197.0
39.10	830.0
43.90	491.0
44.90	496.0
47.00	393.0
48.00	428.0
49.00	2601.0
50.00	11832.0
50.90	3457.0
52.10	154.0
55.00	220.0
55.90	948.0
56.90	1980.0
57.80	100.0
59.90	642.0
61.00	3279.0
62.00	3738.0
63.00	2621.0
63.90	333.0
64.90	491.0
66.90	164.0
67.90	6840.0
69.00	7372.0
69.90	519.0
72.00	335.0
72.90	3643.0
74.00	12382.0
75.00	37408.0
76.00	3292.0
76.90	330.0
77.80	243.0
78.80	2317.0
79.90	673.0
80.90	2177.0
81.90	580.0
86.90	2605.0
87.90	2641.0
90.70	244.0
92.00	2121.0
93.00	3476.0
94.00	8369.0
95.00	71664.0
96.00	4727.0
96.90	150.0
103.80	352.0
104.90	119.0
105.70	346.0
111.90	109.0
115.80	249.0
116.80	605.0
117.80	357.0
118.80	387.0
127.90	269.0
128.80	134.0
129.90	309.0
130.70	143.0
136.70	214.0
140.80	1010.0
142.90	1003.0
145.00	190.0
145.80	101.0
147.60	142.0
149.80	114.0
154.80	179.0
156.80	123.0
159.00	104.0
171.80	662.0
173.80	59472.0
174.90	4427.0
175.80	56776.0
176.80	3892.0

Instrument :
MSVOA_U
ClientSampleId :
BFB043

m/z	Abundance
35.90	462.0
36.90	2415.0
38.00	2055.0
39.10	815.0
43.90	392.0
44.90	473.0
47.00	390.0
48.00	380.0
49.00	2413.0
50.00	10888.0
51.00	3151.0
52.10	152.0
55.00	187.0
55.90	937.0
56.90	1833.0
59.90	583.0
61.00	3087.0
62.00	3379.0
63.00	2403.0
64.00	293.0
65.00	409.0
67.00	151.0
67.90	6506.0
69.00	6874.0
69.90	531.0
72.00	310.0
72.90	3424.0
74.00	11253.0
75.00	34856.0
76.00	2867.0
76.90	365.0
77.80	165.0
78.80	2216.0
79.90	622.0
80.80	1935.0
81.90	551.0
86.90	2470.0
87.90	2335.0
90.80	206.0
92.00	2008.0
92.90	3170.0
94.00	7819.0
95.00	67456.0
96.00	4429.0
97.00	118.0
103.80	327.0
104.90	113.0
105.70	341.0
112.00	110.0
115.80	244.0
116.90	557.0
117.90	339.0
118.70	377.0
123.80	100.0
127.90	241.0
128.80	123.0
129.90	323.0
130.70	127.0
134.80	111.0
136.70	163.0
140.80	977.0
142.80	949.0
144.90	159.0
147.90	141.0
154.80	168.0
156.70	105.0
159.00	122.0
171.80	595.0
173.90	56016.0
174.90	4157.0
175.80	53808.0
176.80	3586.0

Instrument :
MSVOA_U
ClientSampleId :
BFB043