

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
 Data File : VU046284.D
 Acq On : 11 Dec 2021 14:20
 Operator : SY/MD
 Sample : M4982-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CQ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046284.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	75	81	95	rVB	81573	89870	12.30%	1.479%
2	1.919	171	180	193	rVB	67066	86989	11.90%	1.432%
3	2.340	309	311	319	rVB2	427	466	0.06%	0.008%
4	2.571	371	383	402	rBV	141557	235556	32.23%	3.877%
5	2.748	434	438	442	rBV	439	411	0.06%	0.007%
6	2.832	460	464	467	rBV2	616	566	0.08%	0.009%
7	3.054	530	533	537	rVB2	469	363	0.05%	0.006%
8	3.186	570	574	578	rBV2	590	664	0.09%	0.011%
9	3.674	721	726	729	rVB	573	538	0.07%	0.009%
10	3.706	729	736	738	rBV	578	630	0.09%	0.010%
11	3.922	799	803	806	rBV	428	398	0.05%	0.007%
12	4.292	914	918	925	rBV2	335	415	0.06%	0.007%
13	4.636	1010	1025	1062	rBV	78276	223252	30.54%	3.675%
14	4.793	1071	1074	1080	rBV	366	333	0.05%	0.005%
15	4.964	1120	1127	1131	rVB2	679	864	0.12%	0.014%
16	4.996	1131	1137	1140	rBV2	486	462	0.06%	0.008%
17	5.067	1140	1159	1186	rVV	129873	301611	41.26%	4.965%
18	5.420	1265	1269	1275	rVB	553	522	0.07%	0.009%
19	5.485	1285	1289	1292	rBV2	555	394	0.05%	0.006%
20	5.729	1342	1365	1384	rBV2	269186	730938	100.00%	12.031%
21	5.964	1436	1438	1445	rVB3	438	343	0.05%	0.006%
22	6.028	1456	1458	1464	rVB2	398	381	0.05%	0.006%
23	6.057	1464	1467	1471	rVB2	660	484	0.07%	0.008%
24	6.092	1471	1478	1483	rBV2	796	1269	0.17%	0.021%
25	6.253	1506	1528	1553	rBV	229418	433860	59.36%	7.141%
26	6.501	1599	1605	1606	rBV2	425	356	0.05%	0.006%
27	6.533	1606	1615	1632	rVB5	3599	6911	0.95%	0.114%
28	6.600	1632	1636	1640	rBV	374	325	0.04%	0.005%
29	6.693	1650	1665	1693	rVV	172824	337240	46.14%	5.551%
30	6.883	1721	1724	1729	rBV2	507	571	0.08%	0.009%
31	7.156	1805	1809	1813	rBV	317	320	0.04%	0.005%
32	7.189	1814	1819	1825	rVV4	892	1316	0.18%	0.022%
33	7.452	1898	1901	1908	rBV	523	516	0.07%	0.008%
34	7.488	1908	1912	1915	rBV2	402	361	0.05%	0.006%
35	7.568	1925	1937	1959	rBV	98751	171655	23.48%	2.825%
36	7.845	2020	2023	2027	rBV	405	361	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
 Data File : VU046284.D
 Acq On : 11 Dec 2021 14:20
 Operator : SY/MD
 Sample : M4982-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CQ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.899	2027	2040	2057	rBV	325788	566502	77.50%	9.325%
38	8.099	2099	2102	2106	rVB	479	369	0.05%	0.006%
39	8.182	2117	2128	2144	rBV	69911	114622	15.68%	1.887%
40	8.311	2164	2168	2172	rBV2	491	366	0.05%	0.006%
41	8.365	2179	2185	2191	rVB	573	725	0.10%	0.012%
42	8.436	2203	2207	2210	rBV	566	498	0.07%	0.008%
43	8.472	2214	2218	2227	rVB2	1065	1664	0.23%	0.027%
44	8.555	2241	2244	2249	rBV	450	374	0.05%	0.006%
45	8.636	2257	2269	2298	rBV	264046	453303	62.02%	7.461%
46	8.812	2320	2324	2327	rBV	522	405	0.06%	0.007%
47	8.848	2331	2335	2339	rVV	516	394	0.05%	0.006%
48	8.902	2348	2352	2359	rBV	487	565	0.08%	0.009%
49	9.063	2398	2402	2406	rVB	634	439	0.06%	0.007%
50	9.163	2431	2433	2440	rVB2	550	547	0.07%	0.009%
51	9.420	2499	2513	2536	rBV	340307	563256	77.06%	9.271%
52	9.568	2555	2559	2563	rBV2	741	762	0.10%	0.013%
53	9.697	2592	2599	2607	rVB3	2019	3147	0.43%	0.052%
54	9.774	2621	2623	2631	rVB	440	391	0.05%	0.006%
55	10.012	2693	2697	2701	rBV	330	319	0.04%	0.005%
56	10.108	2719	2727	2734	rBV3	756	1172	0.16%	0.019%
57	10.192	2750	2753	2759	rBV	435	416	0.06%	0.007%
58	10.262	2768	2775	2778	rBV	548	734	0.10%	0.012%
59	10.317	2789	2792	2798	rVB2	544	563	0.08%	0.009%
60	10.346	2798	2801	2808	rVB2	561	640	0.09%	0.011%
61	10.381	2808	2812	2814	rBV	511	423	0.06%	0.007%
62	10.668	2894	2901	2908	rBV4	1168	1857	0.25%	0.031%
63	10.758	2914	2929	2948	rBV	278097	445941	61.01%	7.340%
64	10.896	2965	2972	2980	rVB4	1313	1924	0.26%	0.032%
65	10.996	2999	3003	3010	rBV2	511	669	0.09%	0.011%
66	11.118	3037	3041	3048	rVB4	2728	3267	0.45%	0.054%
67	11.240	3073	3079	3080	rBV2	404	411	0.06%	0.007%
68	11.372	3117	3120	3124	rBV3	596	586	0.08%	0.010%
69	11.417	3128	3134	3139	rVV3	1168	1705	0.23%	0.028%
70	11.471	3143	3151	3159	rVB6	2212	3684	0.50%	0.061%
71	11.561	3175	3179	3183	rBV2	527	466	0.06%	0.008%
72	11.616	3191	3196	3202	rBV2	512	640	0.09%	0.011%
73	11.703	3216	3223	3226	rBV5	1117	1433	0.20%	0.024%
74	11.812	3245	3257	3272	rBV	399483	620423	84.88%	10.212%
75	11.905	3283	3286	3291	rBV4	715	630	0.09%	0.010%
76	11.976	3304	3308	3312	rVB4	891	703	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
 Data File : VU046284.D
 Acq On : 11 Dec 2021 14:20
 Operator : SY/MD
 Sample : M4982-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CQ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	12.127	3353	3355	3359	rBV2	525	424	0.06%	0.007%
78	12.195	3363	3376	3391	rVV	378757	601748	82.33%	9.905%
79	12.275	3397	3401	3405	rBV3	633	553	0.08%	0.009%
80	12.327	3410	3417	3426	rBV4	4972	7114	0.97%	0.117%
81	12.401	3437	3440	3443	rBV2	415	337	0.05%	0.006%
82	12.655	3513	3519	3523	rBV3	756	868	0.12%	0.014%
83	12.767	3549	3554	3558	rBV3	617	811	0.11%	0.013%
84	12.905	3590	3597	3600	rBV2	657	863	0.12%	0.014%
85	12.957	3611	3613	3617	rVB2	621	406	0.06%	0.007%
86	12.979	3618	3620	3626	rVB3	748	588	0.08%	0.010%
87	13.005	3626	3628	3632	rBV2	709	503	0.07%	0.008%
88	13.137	3667	3669	3672	rVB4	686	363	0.05%	0.006%
89	13.410	3750	3754	3755	rBV	429	350	0.05%	0.006%
90	13.433	3755	3761	3767	rVB4	1843	2514	0.34%	0.041%
91	14.040	3946	3950	3956	rBV3	448	571	0.08%	0.009%
92	14.089	3957	3965	3975	rVV	7279	10592	1.45%	0.174%
93	14.452	4071	4078	4085	rVB6	1907	2584	0.35%	0.043%
94	14.651	4137	4140	4143	rVB	815	527	0.07%	0.009%
95	15.227	4310	4319	4326	rBV	3882	6085	0.83%	0.100%
96	15.301	4339	4342	4349	rBV3	618	487	0.07%	0.008%
97	15.404	4367	4374	4382	rBB4	2701	4053	0.55%	0.067%
98	15.899	4525	4528	4529	rBV	582	359	0.05%	0.006%
99	16.262	4637	4641	4646	rVB4	2401	2167	0.30%	0.036%
100	16.413	4683	4688	4694	rVB5	1750	2014	0.28%	0.033%




Sum of corrected areas: 6075327

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
Data File : VU046284.D
Acq On : 11 Dec 2021 14:20
Operator : SY/MD
Sample : M4982-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CQ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

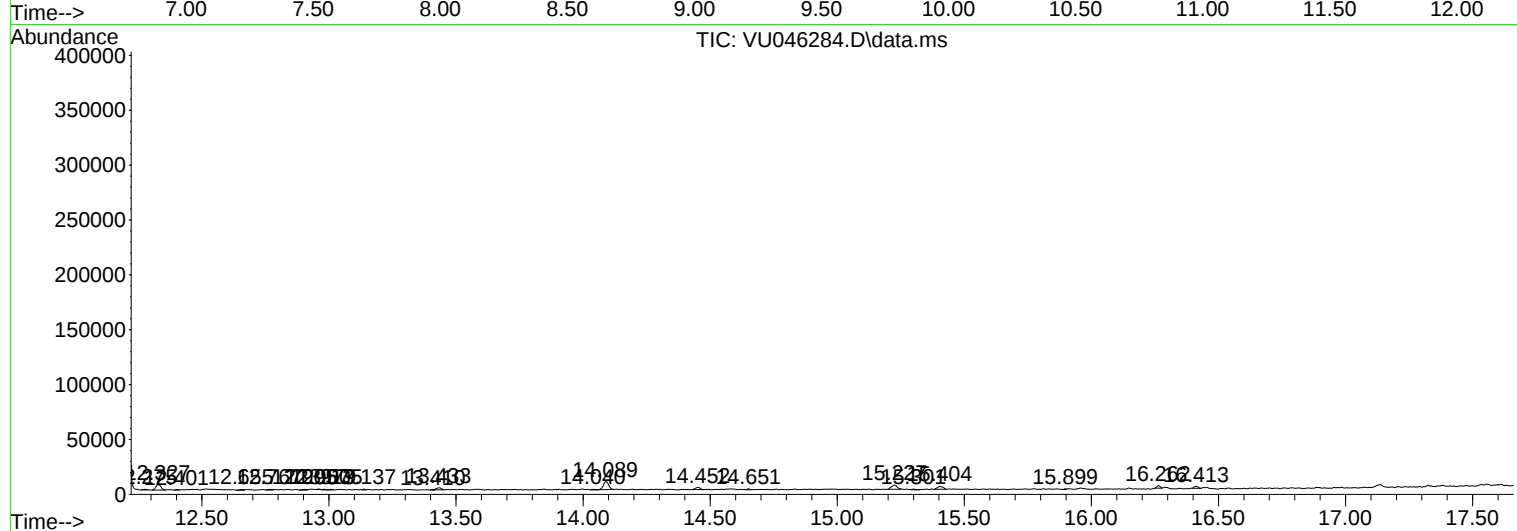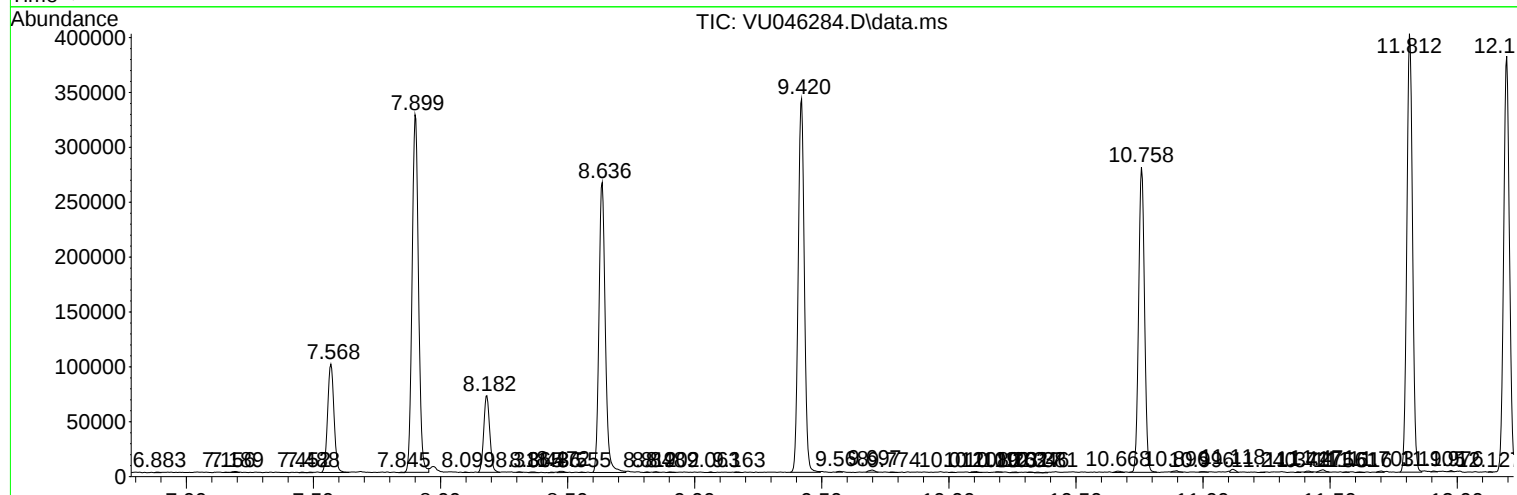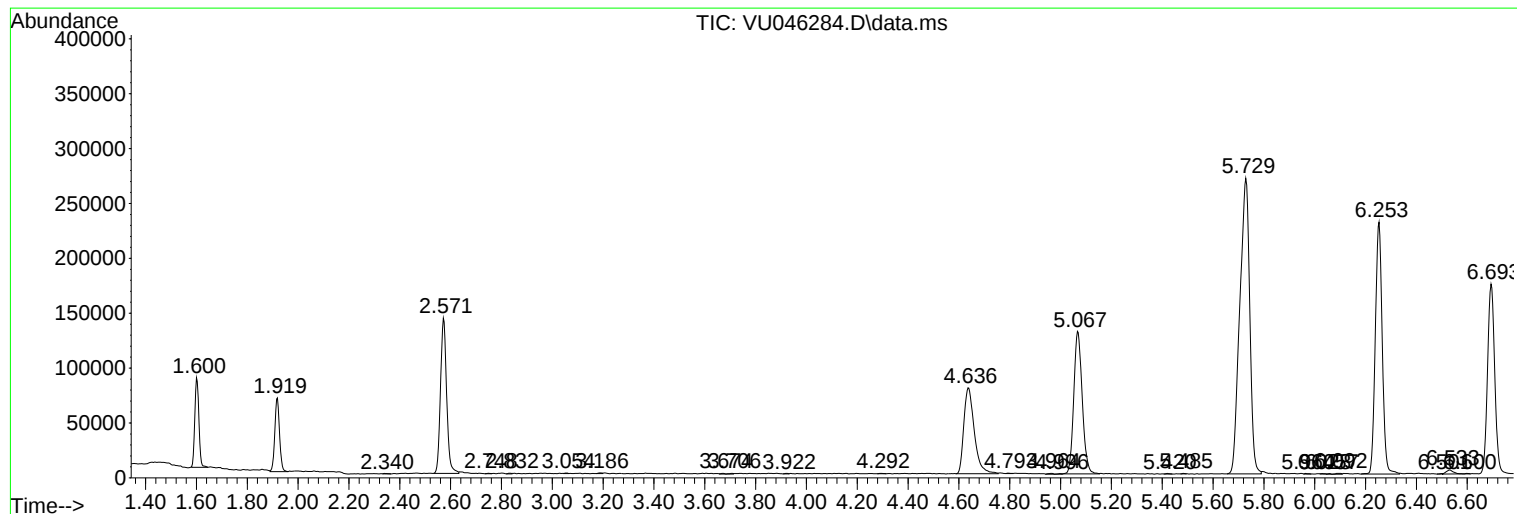

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
Data File : VU046284.D
Acq On : 11 Dec 2021 14:20
Operator : SY/MD
Sample : M4982-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CQ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
Data File : VU046284.D
Acq On : 11 Dec 2021 14:20
Operator : SY/MD
Sample : M4982-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CQ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc