

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
 Data File : VU046285.D
 Acq On : 11 Dec 2021 14:42
 Operator : SY/MD
 Sample : M4982-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046285.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	75	81	97	rVB	84048	92758	12.72%	1.552%
2	1.919	172	180	196	rVB	65561	83937	11.51%	1.404%
3	2.311	300	302	310	rVB2	481	448	0.06%	0.007%
4	2.411	330	333	336	rBV2	327	267	0.04%	0.004%
5	2.571	372	383	411	rVB	139134	236395	32.41%	3.955%
6	3.176	567	571	576	rBV3	610	752	0.10%	0.013%
7	3.269	597	600	603	rVB	496	262	0.04%	0.004%
8	3.308	608	612	618	rBV2	369	501	0.07%	0.008%
9	3.543	682	685	692	rVB2	319	309	0.04%	0.005%
10	3.742	744	747	752	rBV	433	359	0.05%	0.006%
11	3.777	755	758	761	rVB	531	329	0.05%	0.006%
12	3.932	802	806	808	rBV	440	357	0.05%	0.006%
13	3.967	814	817	822	rBV	424	374	0.05%	0.006%
14	4.211	890	893	896	rBV	409	330	0.05%	0.006%
15	4.327	925	929	934	rBV	272	361	0.05%	0.006%
16	4.507	981	985	987	rBV	580	529	0.07%	0.009%
17	4.636	1010	1025	1053	rBV	77031	216836	29.73%	3.627%
18	4.919	1110	1113	1116	rBV	344	282	0.04%	0.005%
19	5.067	1143	1159	1185	rVV	130096	303843	41.66%	5.083%
20	5.237	1208	1212	1213	rBV2	426	304	0.04%	0.005%
21	5.546	1304	1308	1312	rBV	496	445	0.06%	0.007%
22	5.600	1322	1325	1330	rVB	434	330	0.05%	0.006%
23	5.729	1343	1365	1388	rBV2	266555	729338	100.00%	12.201%
24	5.851	1401	1403	1407	rVB3	568	435	0.06%	0.007%
25	5.893	1412	1416	1420	rVB2	797	695	0.10%	0.012%
26	5.922	1420	1425	1431	rBV3	709	980	0.13%	0.016%
27	5.951	1431	1434	1437	rBV	431	335	0.05%	0.006%
28	6.179	1502	1505	1510	rVB	638	521	0.07%	0.009%
29	6.253	1514	1528	1560	rVV	222156	423199	58.03%	7.080%
30	6.546	1606	1619	1631	rBV3	18636	35757	4.90%	0.598%
31	6.694	1651	1665	1685	rBV	172014	332795	45.63%	5.567%
32	6.861	1711	1717	1720	rBV2	347	388	0.05%	0.006%
33	7.112	1791	1795	1800	rBV2	494	403	0.06%	0.007%
34	7.185	1811	1818	1826	rBV3	836	1331	0.18%	0.022%
35	7.526	1921	1924	1925	rBV	526	305	0.04%	0.005%
36	7.568	1925	1937	1955	rVB	99791	170635	23.40%	2.855%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
 Data File : VU046285.D
 Acq On : 11 Dec 2021 14:42
 Operator : SY/MD
 Sample : M4982-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.690	1971	1975	1977	rBV2	440	387	0.05%	0.006%
38	7.745	1987	1992	1995	rBV2	354	399	0.05%	0.007%
39	7.899	2026	2040	2058	rBV	322937	560892	76.90%	9.383%
40	7.970	2058	2062	2071	rVB	4440	6343	0.87%	0.106%
41	8.182	2116	2128	2148	rBV	68934	115501	15.84%	1.932%
42	8.475	2209	2219	2228	rBV3	2235	3937	0.54%	0.066%
43	8.636	2256	2269	2294	rBV	262066	444032	60.88%	7.428%
44	8.783	2312	2315	2319	rVB2	448	336	0.05%	0.006%
45	8.809	2319	2323	2325	rBV	388	338	0.05%	0.006%
46	8.902	2348	2352	2355	rBV2	466	509	0.07%	0.009%
47	9.420	2500	2513	2536	rBV	338241	554673	76.05%	9.279%
48	9.674	2587	2592	2594	rBV2	368	352	0.05%	0.006%
49	9.700	2594	2600	2607	rVB4	1125	1452	0.20%	0.024%
50	9.861	2647	2650	2654	rBV2	332	310	0.04%	0.005%
51	9.902	2658	2663	2667	rBV2	429	431	0.06%	0.007%
52	9.941	2667	2675	2679	rBV	527	643	0.09%	0.011%
53	9.983	2686	2688	2694	rVB2	395	301	0.04%	0.005%
54	10.018	2694	2699	2701	rBV	365	278	0.04%	0.005%
55	10.214	2756	2760	2765	rBV2	457	496	0.07%	0.008%
56	10.365	2804	2807	2810	rBV2	367	264	0.04%	0.004%
57	10.533	2856	2859	2864	rVB2	540	389	0.05%	0.007%
58	10.565	2864	2869	2871	rBV2	324	316	0.04%	0.005%
59	10.629	2886	2889	2894	rBV	378	337	0.05%	0.006%
60	10.677	2899	2904	2912	rVV4	776	1118	0.15%	0.019%
61	10.709	2912	2914	2916	rVV	454	281	0.04%	0.005%
62	10.758	2916	2929	2949	rVB	279181	442204	60.63%	7.398%
63	10.893	2964	2971	2983	rVB2	2480	3569	0.49%	0.060%
64	10.992	2998	3002	3009	rVB2	692	718	0.10%	0.012%
65	11.092	3029	3033	3035	rBV2	402	335	0.05%	0.006%
66	11.169	3053	3057	3058	rBV	400	272	0.04%	0.005%
67	11.291	3092	3095	3099	rBV	460	296	0.04%	0.005%
68	11.372	3116	3120	3124	rBV2	383	377	0.05%	0.006%
69	11.430	3134	3138	3142	rVB2	332	334	0.05%	0.006%
70	11.465	3142	3149	3150	rBV2	940	895	0.12%	0.015%
71	11.549	3172	3175	3181	rVB	396	371	0.05%	0.006%
72	11.716	3225	3227	3229	rBV	461	289	0.04%	0.005%
73	11.729	3229	3231	3234	rVV	479	334	0.05%	0.006%
74	11.748	3234	3237	3241	rVV3	812	724	0.10%	0.012%
75	11.767	3241	3243	3245	rVV	648	447	0.06%	0.007%
76	11.812	3245	3257	3279	rVV	381878	593925	81.43%	9.936%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
 Data File : VU046285.D
 Acq On : 11 Dec 2021 14:42
 Operator : SY/MD
 Sample : M4982-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.893	3279	3282	3285	rVV2	317	262	0.04%	0.004%
78	11.918	3288	3290	3294	rVB	461	338	0.05%	0.006%
79	11.947	3294	3299	3302	rBV2	522	589	0.08%	0.010%
80	11.970	3302	3306	3312	rVB2	532	509	0.07%	0.009%
81	12.134	3352	3357	3363	rBV2	466	587	0.08%	0.010%
82	12.195	3363	3376	3390	rBV	372609	585225	80.24%	9.790%
83	12.330	3413	3418	3427	rVB6	1406	1605	0.22%	0.027%
84	12.407	3439	3442	3449	rVB2	232	288	0.04%	0.005%
85	12.536	3479	3482	3485	rBV2	418	335	0.05%	0.006%
86	12.632	3503	3512	3516	rBV2	305	611	0.08%	0.010%
87	12.706	3532	3535	3543	rVB2	543	618	0.08%	0.010%
88	12.745	3543	3547	3549	rBV2	369	336	0.05%	0.006%
89	12.767	3550	3554	3556	rBV2	719	554	0.08%	0.009%
90	13.433	3756	3761	3764	rBV2	710	641	0.09%	0.011%
91	13.629	3814	3822	3826	rBV2	495	692	0.09%	0.012%
92	13.658	3826	3831	3835	rVV2	354	418	0.06%	0.007%
93	13.983	3924	3932	3934	rBV2	546	662	0.09%	0.011%
94	14.008	3937	3940	3943	rVB	501	336	0.05%	0.006%
95	14.037	3946	3949	3953	rVB2	435	332	0.05%	0.006%
96	14.092	3953	3966	3973	rBV2	1907	3417	0.47%	0.057%
97	14.352	4043	4047	4050	rBV2	509	483	0.07%	0.008%
98	15.404	4371	4374	4378	rVB2	990	804	0.11%	0.013%
99	15.484	4396	4399	4403	rBV2	648	582	0.08%	0.010%
100	15.552	4417	4420	4424	rBV2	655	585	0.08%	0.010%




Sum of corrected areas: 5977639

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
Data File : VU046285.D
Acq On : 11 Dec 2021 14:42
Operator : SY/MD
Sample : M4982-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

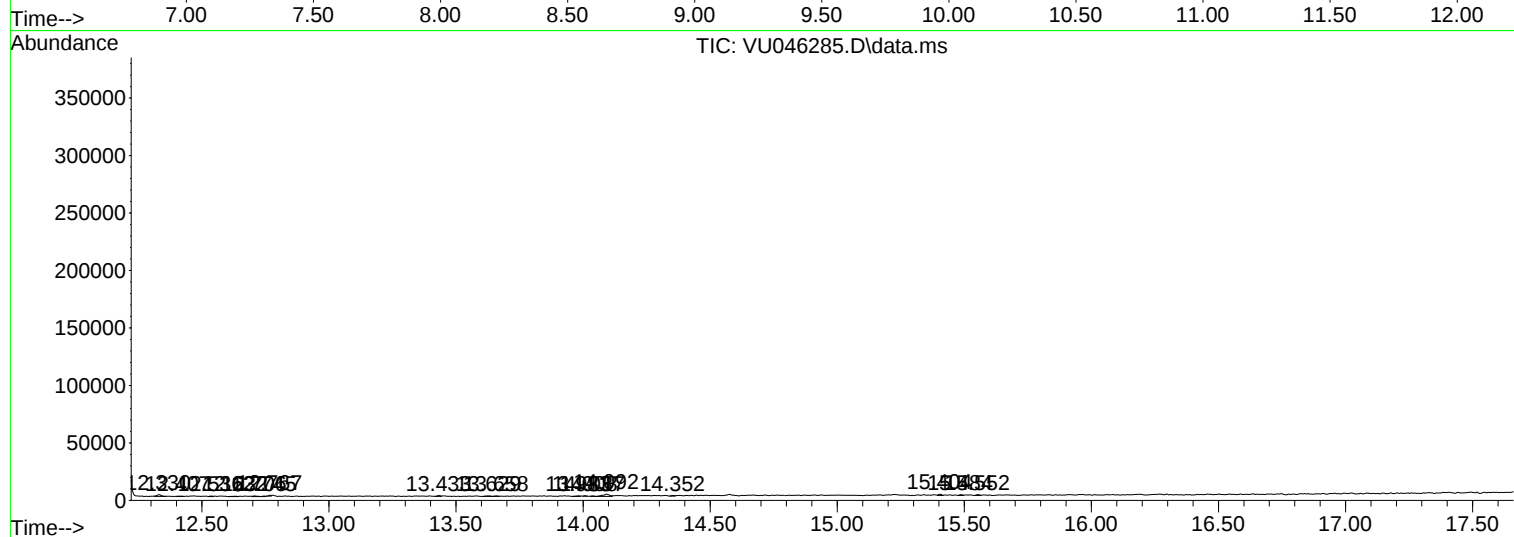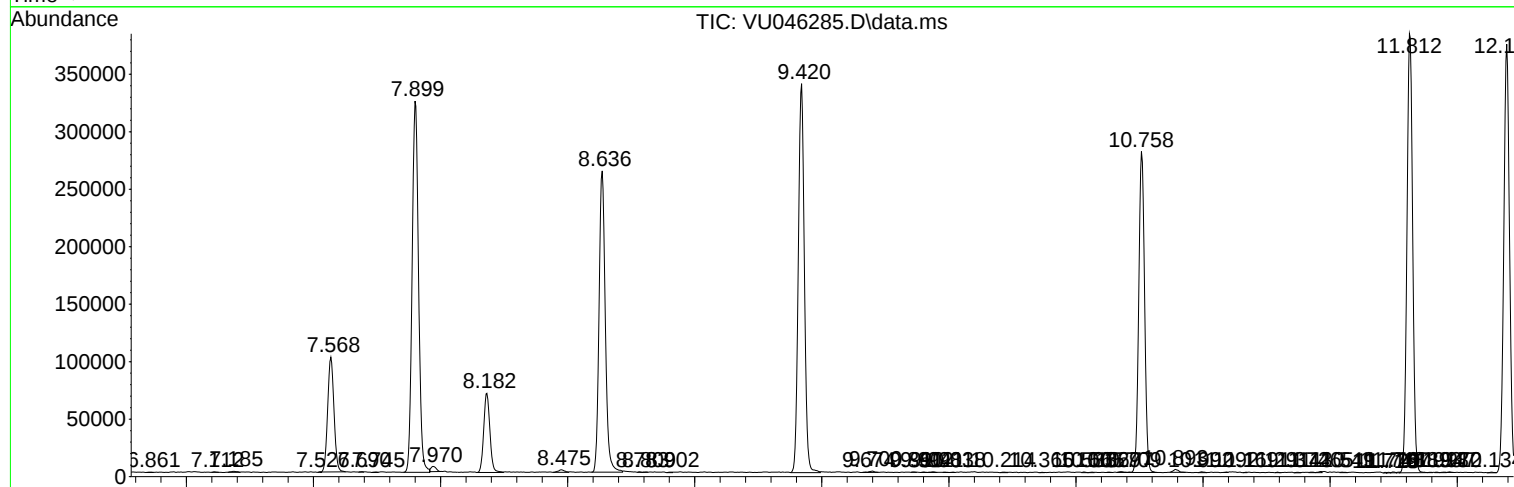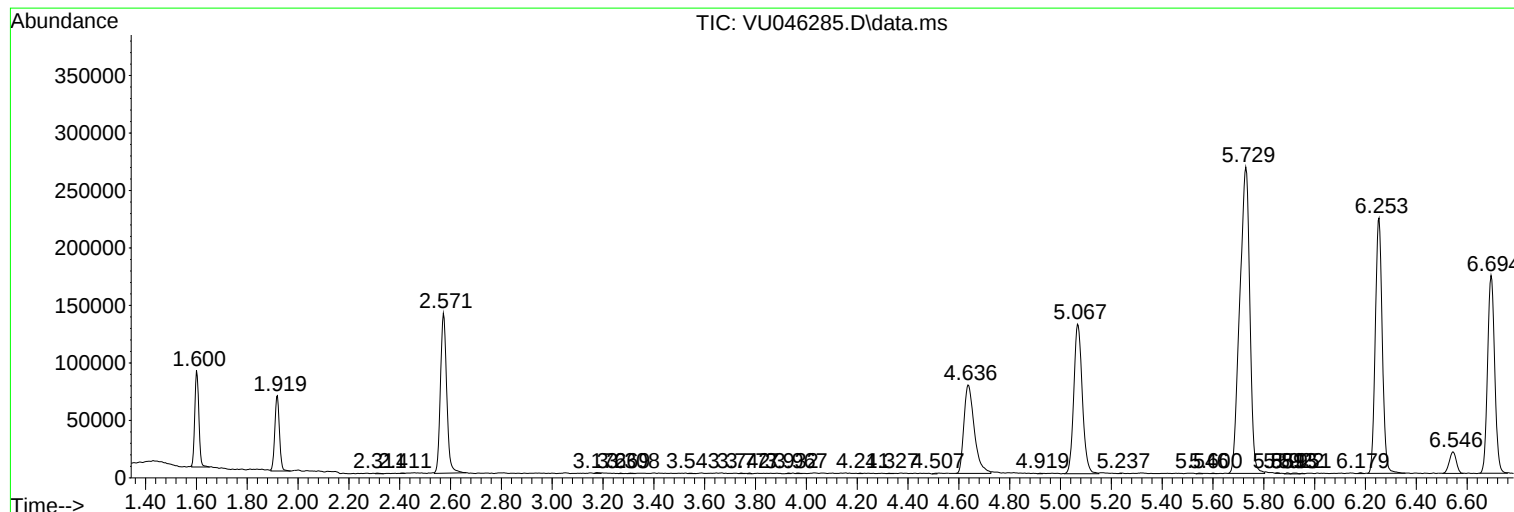

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
Data File : VU046285.D
Acq On : 11 Dec 2021 14:42
Operator : SY/MD
Sample : M4982-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
Data File : VU046285.D
Acq On : 11 Dec 2021 14:42
Operator : SY/MD
Sample : M4982-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc