

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
 Data File : VU046287.D
 Acq On : 11 Dec 2021 15:27
 Operator : SY/MD
 Sample : M4943-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M

Title : VOC Analysis

Signal : TIC: VU046287.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	75	81	94	rVB	84159	92259	12.58%	1.566%
2	1.916	172	179	191	rVB	67256	84999	11.59%	1.443%
3	2.195	263	266	270	rVB	536	398	0.05%	0.007%
4	2.240	276	280	282	rBV	456	330	0.05%	0.006%
5	2.572	371	383	407	rBV	142777	240540	32.80%	4.082%
6	2.681	413	417	423	rVB2	622	629	0.09%	0.011%
7	2.748	435	438	441	rBV	478	361	0.05%	0.006%
8	2.787	446	450	453	rBV2	345	358	0.05%	0.006%
9	2.867	472	475	481	rVB	396	354	0.05%	0.006%
10	2.964	500	505	509	rVB2	551	691	0.09%	0.012%
11	3.047	526	531	540	rVV3	1243	1658	0.23%	0.028%
12	3.189	563	575	591	rVB2	2559	6213	0.85%	0.105%
13	3.388	630	637	640	rBV	356	390	0.05%	0.007%
14	3.716	736	739	742	rBV2	470	316	0.04%	0.005%
15	3.906	794	798	804	rBV	534	602	0.08%	0.010%
16	4.002	824	828	830	rBV	367	307	0.04%	0.005%
17	4.057	841	845	848	rBV	479	347	0.05%	0.006%
18	4.205	887	891	893	rBV	372	292	0.04%	0.005%
19	4.346	932	935	940	rVB	315	288	0.04%	0.005%
20	4.375	941	944	951	rBV	376	454	0.06%	0.008%
21	4.549	990	998	1001	rBV2	395	499	0.07%	0.008%
22	4.571	1001	1005	1010	rBV2	336	360	0.05%	0.006%
23	4.636	1010	1025	1058	rBV	82161	228670	31.18%	3.881%
24	5.067	1143	1159	1180	rBV	132358	304307	41.50%	5.164%
25	5.594	1318	1323	1325	rBV	385	311	0.04%	0.005%
26	5.642	1331	1338	1342	rBV	415	577	0.08%	0.010%
27	5.729	1342	1365	1387	rBV2	267310	733287	100.00%	12.445%
28	5.864	1401	1407	1410	rBV	552	520	0.07%	0.009%
29	6.086	1472	1476	1481	rBV2	427	449	0.06%	0.008%
30	6.131	1488	1490	1495	rVB2	437	293	0.04%	0.005%
31	6.195	1506	1510	1513	rBV	470	440	0.06%	0.007%
32	6.253	1515	1528	1559	rVV	208153	394974	53.86%	6.703%
33	6.452	1586	1590	1596	rBB2	427	381	0.05%	0.006%
34	6.533	1606	1615	1624	rBV5	3955	7409	1.01%	0.126%
35	6.694	1651	1665	1685	rVV	172727	337471	46.02%	5.727%
36	6.980	1750	1754	1758	rBV	379	339	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
 Data File : VU046287.D
 Acq On : 11 Dec 2021 15:27
 Operator : SY/MD
 Sample : M4943-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.005	1758	1762	1765	rBV2	358	309	0.04%	0.005%
38	7.179	1811	1816	1817	rBV	587	450	0.06%	0.008%
39	7.269	1838	1844	1845	rBV2	445	378	0.05%	0.006%
40	7.568	1924	1937	1954	rBV	98044	171328	23.36%	2.908%
41	7.697	1974	1977	1982	rVB2	464	410	0.06%	0.007%
42	7.899	2026	2040	2058	rBV	328160	563667	76.87%	9.566%
43	8.063	2087	2091	2098	rVB2	593	773	0.11%	0.013%
44	8.182	2116	2128	2147	rBV	68397	114730	15.65%	1.947%
45	8.279	2155	2158	2162	rBV	395	321	0.04%	0.005%
46	8.308	2162	2167	2172	rVV3	423	486	0.07%	0.008%
47	8.369	2182	2186	2191	rVB	586	591	0.08%	0.010%
48	8.401	2191	2196	2198	rBV	411	398	0.05%	0.007%
49	8.417	2198	2201	2204	rBV	630	396	0.05%	0.007%
50	8.517	2225	2232	2235	rBV	307	433	0.06%	0.007%
51	8.636	2256	2269	2297	rBV	265330	454082	61.92%	7.706%
52	8.915	2346	2356	2363	rBV3	1598	2967	0.40%	0.050%
53	8.983	2374	2377	2381	rVV2	310	304	0.04%	0.005%
54	9.057	2395	2400	2403	rBV2	427	464	0.06%	0.008%
55	9.301	2473	2476	2480	rBV	444	368	0.05%	0.006%
56	9.420	2499	2513	2539	rBV	321043	524108	71.47%	8.895%
57	9.697	2592	2599	2606	rVB3	958	1177	0.16%	0.020%
58	9.986	2682	2689	2693	rVB	597	659	0.09%	0.011%
59	10.034	2699	2704	2712	rBV	408	623	0.08%	0.011%
60	10.211	2755	2759	2763	rBV2	286	306	0.04%	0.005%
61	10.234	2764	2766	2773	rVB	430	372	0.05%	0.006%
62	10.359	2800	2805	2806	rBV2	318	287	0.04%	0.005%
63	10.549	2861	2864	2869	rVB2	334	334	0.05%	0.006%
64	10.581	2869	2874	2877	rBV	420	478	0.07%	0.008%
65	10.674	2901	2903	2907	rVB2	633	392	0.05%	0.007%
66	10.758	2916	2929	2944	rBV	279010	447272	61.00%	7.591%
67	10.938	2979	2985	2988	rBV2	698	635	0.09%	0.011%
68	11.128	3042	3044	3050	rVB2	400	287	0.04%	0.005%
69	11.439	3136	3141	3143	rBV2	554	559	0.08%	0.009%
70	11.536	3166	3171	3174	rBV2	393	409	0.06%	0.007%
71	11.812	3245	3257	3278	rVB	355374	554048	75.56%	9.403%
72	11.893	3278	3282	3284	rBV2	581	413	0.06%	0.007%
73	12.031	3322	3325	3330	rBV2	314	351	0.05%	0.006%
74	12.073	3334	3338	3340	rBV	357	322	0.04%	0.005%
75	12.134	3351	3357	3362	rVB	546	691	0.09%	0.012%
76	12.195	3362	3376	3403	rVB	369199	592052	80.74%	10.048%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
 Data File : VU046287.D
 Acq On : 11 Dec 2021 15:27
 Operator : SY/MD
 Sample : M4943-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	12.304	3403	3410	3413	rBV2	497	529	0.07%	0.009%
78	12.333	3414	3419	3422	rBV3	456	430	0.06%	0.007%
79	12.426	3444	3448	3451	rBV	621	492	0.07%	0.008%
80	12.758	3546	3551	3553	rBV	752	678	0.09%	0.012%
81	12.841	3575	3577	3584	rVB2	407	347	0.05%	0.006%
82	13.407	3750	3753	3759	rVB	566	466	0.06%	0.008%
83	13.478	3770	3775	3778	rBV2	511	557	0.08%	0.009%
84	13.536	3788	3793	3797	rBV2	326	374	0.05%	0.006%
85	13.565	3797	3802	3805	rBV	435	380	0.05%	0.006%
86	14.015	3935	3942	3947	rBV2	543	628	0.09%	0.011%
87	14.163	3985	3988	3994	rBV	417	390	0.05%	0.007%
88	14.195	3994	3998	4003	rVV2	385	397	0.05%	0.007%
89	14.356	4043	4048	4054	rBV	484	557	0.08%	0.009%
90	14.696	4150	4154	4158	rBV2	375	348	0.05%	0.006%
91	14.841	4196	4199	4202	rBV2	385	305	0.04%	0.005%
92	14.857	4202	4204	4208	rVV	453	366	0.05%	0.006%
93	14.893	4211	4215	4217	rBV2	458	323	0.04%	0.005%
94	14.973	4237	4240	4246	rVB	522	490	0.07%	0.008%
95	15.385	4364	4368	4370	rBV2	628	444	0.06%	0.008%
96	15.587	4428	4431	4440	rBV	343	439	0.06%	0.007%
97	15.893	4522	4526	4529	rBV3	744	547	0.07%	0.009%
98	16.224	4625	4629	4635	rBV2	627	901	0.12%	0.015%
99	16.526	4720	4723	4728	rBV2	679	516	0.07%	0.009%
100	16.555	4728	4732	4739	rVV3	696	807	0.11%	0.014%




Sum of corrected areas: 5892414

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
Data File : VU046287.D
Acq On : 11 Dec 2021 15:27
Operator : SY/MD
Sample : M4943-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

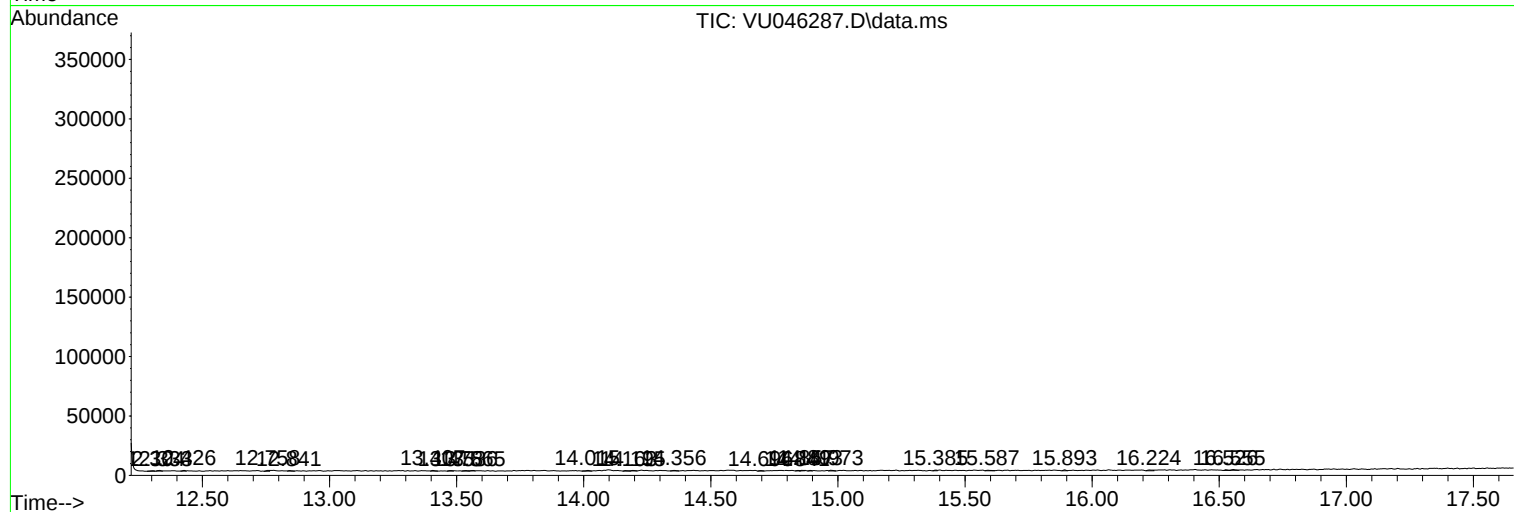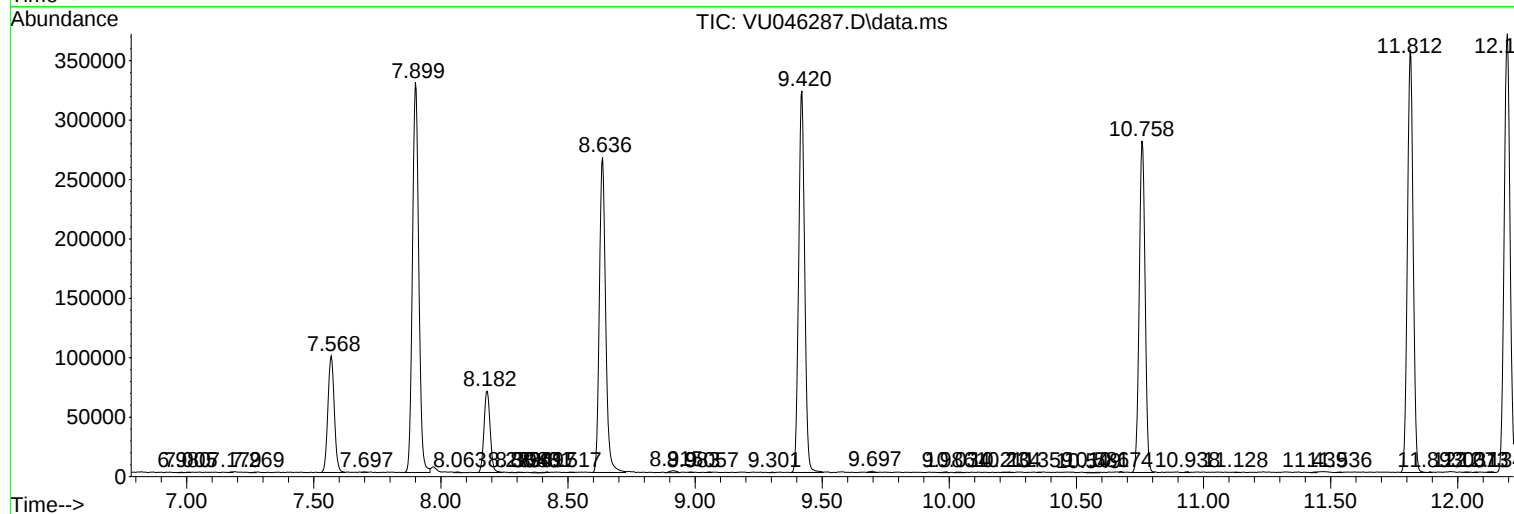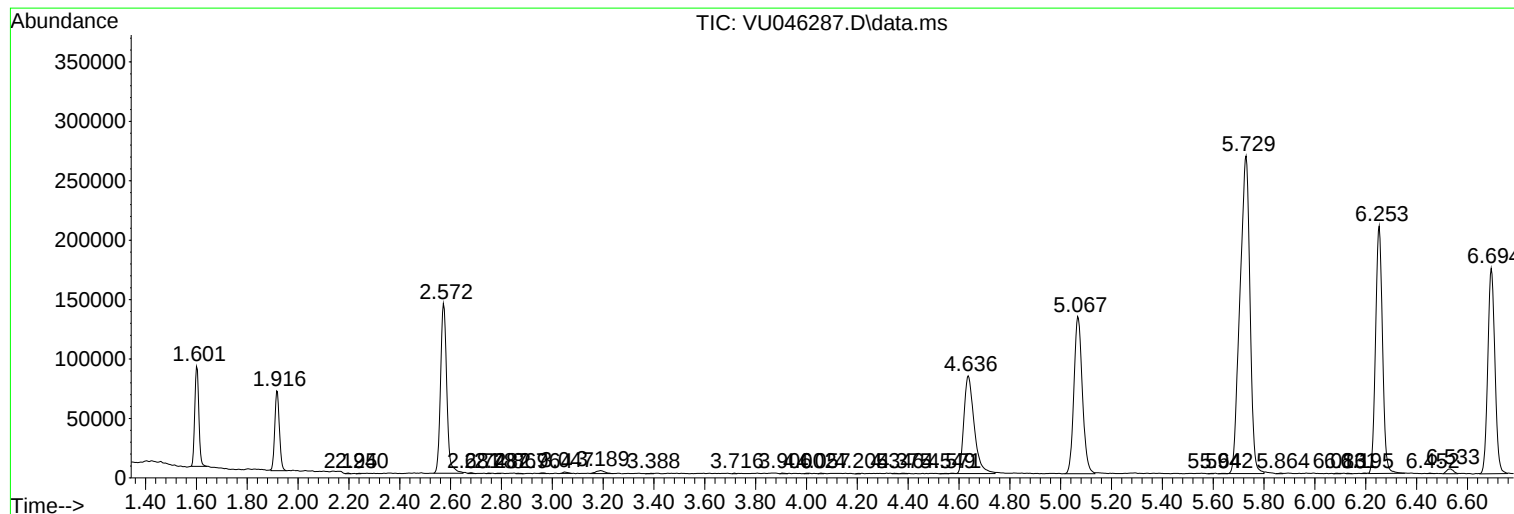

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
Data File : VU046287.D
Acq On : 11 Dec 2021 15:27
Operator : SY/MD
Sample : M4943-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
Data File : VU046287.D
Acq On : 11 Dec 2021 15:27
Operator : SY/MD
Sample : M4943-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------