

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
 Data File : VU046299.D
 Acq On : 11 Dec 2021 19:57
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK009

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046299.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	93	rBV	74390	81184	12.80%	1.623%
2	1.916	171	179	196	rVB	59325	76652	12.09%	1.532%
3	2.337	307	310	313	rBV2	447	366	0.06%	0.007%
4	2.385	319	325	330	rBV2	310	383	0.06%	0.008%
5	2.443	339	343	349	rBV2	564	700	0.11%	0.014%
6	2.571	371	383	414	rBV	120123	203688	32.13%	4.072%
7	2.838	463	466	470	rVB2	434	313	0.05%	0.006%
8	2.948	497	500	503	rBV2	451	313	0.05%	0.006%
9	3.051	525	532	542	rVB4	2078	3551	0.56%	0.071%
10	3.157	560	565	570	rBV2	375	483	0.08%	0.010%
11	3.346	620	624	626	rBV	385	337	0.05%	0.007%
12	3.427	645	649	651	rBV	356	280	0.04%	0.006%
13	3.533	678	682	686	rBV2	493	436	0.07%	0.009%
14	3.655	716	720	723	rBV2	409	274	0.04%	0.005%
15	3.674	723	726	731	rBV	394	396	0.06%	0.008%
16	4.070	846	849	854	rBV2	281	309	0.05%	0.006%
17	4.452	965	968	973	rBV	397	370	0.06%	0.007%
18	4.552	996	999	1003	rBV	320	291	0.05%	0.006%
19	4.639	1011	1026	1059	rBV	66515	191325	30.18%	3.825%
20	5.070	1144	1160	1182	rVV2	108649	263989	41.64%	5.277%
21	5.269	1218	1222	1227	rBV2	274	350	0.06%	0.007%
22	5.298	1227	1231	1235	rVB3	579	571	0.09%	0.011%
23	5.321	1235	1238	1241	rBV	429	312	0.05%	0.006%
24	5.449	1275	1278	1282	rVB	458	311	0.05%	0.006%
25	5.552	1308	1310	1315	rVB	418	274	0.04%	0.005%
26	5.584	1315	1320	1323	rBV2	318	291	0.05%	0.006%
27	5.729	1343	1365	1387	rBV2	229401	634026	100.00%	12.675%
28	5.938	1427	1430	1434	rBV	442	289	0.05%	0.006%
29	5.986	1439	1445	1448	rBV2	378	447	0.07%	0.009%
30	6.031	1454	1459	1462	rBV2	356	305	0.05%	0.006%
31	6.253	1512	1528	1550	rBV	177696	336467	53.07%	6.726%
32	6.452	1587	1590	1594	rVV	460	350	0.06%	0.007%
33	6.530	1606	1614	1624	rVB3	2990	5194	0.82%	0.104%
34	6.636	1641	1647	1649	rBV2	255	299	0.05%	0.006%
35	6.693	1650	1665	1686	rVV	150914	290730	45.85%	5.812%
36	6.806	1697	1700	1701	rBV	595	344	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
 Data File : VU046299.D
 Acq On : 11 Dec 2021 19:57
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK009

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.973	1746	1752	1755	rBV2	281	351	0.06%	0.007%
38	7.073	1780	1783	1788	rBV2	568	635	0.10%	0.013%
39	7.173	1811	1814	1816	rBV2	516	378	0.06%	0.008%
40	7.230	1825	1832	1834	rBV	398	466	0.07%	0.009%
41	7.337	1861	1865	1869	rVB	415	305	0.05%	0.006%
42	7.365	1869	1874	1877	rBV	435	366	0.06%	0.007%
43	7.436	1890	1896	1899	rBV2	276	379	0.06%	0.008%
44	7.475	1904	1908	1915	rVV	446	579	0.09%	0.012%
45	7.568	1925	1937	1951	rVB	80608	139715	22.04%	2.793%
46	7.645	1956	1961	1963	rBV	329	264	0.04%	0.005%
47	7.899	2024	2040	2057	rBV	269889	472954	74.60%	9.455%
48	8.182	2117	2128	2142	rVV	58256	95408	15.05%	1.907%
49	8.417	2198	2201	2205	rBV	328	267	0.04%	0.005%
50	8.478	2214	2220	2223	rBV2	341	396	0.06%	0.008%
51	8.520	2228	2233	2237	rBV2	487	587	0.09%	0.012%
52	8.636	2257	2269	2296	rBV	224296	385587	60.82%	7.708%
53	8.899	2347	2351	2354	rBV2	454	401	0.06%	0.008%
54	8.973	2368	2374	2381	rBV2	579	805	0.13%	0.016%
55	9.144	2424	2427	2431	rBV2	493	448	0.07%	0.009%
56	9.246	2455	2459	2464	rBV2	359	331	0.05%	0.007%
57	9.420	2500	2513	2530	rBV	274646	452005	71.29%	9.036%
58	9.655	2582	2586	2590	rBV	336	333	0.05%	0.007%
59	9.777	2619	2624	2626	rBV	463	411	0.06%	0.008%
60	9.822	2635	2638	2640	rBV	480	331	0.05%	0.007%
61	10.041	2698	2706	2711	rBV	482	632	0.10%	0.013%
62	10.066	2711	2714	2717	rBV2	368	313	0.05%	0.006%
63	10.349	2799	2802	2805	rVB	502	342	0.05%	0.007%
64	10.433	2824	2828	2833	rBV2	387	442	0.07%	0.009%
65	10.459	2834	2836	2842	rVB	523	410	0.06%	0.008%
66	10.491	2842	2846	2850	rBV	421	474	0.07%	0.009%
67	10.590	2875	2877	2881	rBV	432	253	0.04%	0.005%
68	10.616	2881	2885	2888	rVB	566	490	0.08%	0.010%
69	10.645	2888	2894	2899	rBV2	529	688	0.11%	0.014%
70	10.758	2916	2929	2945	rVB	241548	383255	60.45%	7.661%
71	11.025	3009	3012	3018	rVB2	586	618	0.10%	0.012%
72	11.115	3037	3040	3046	rVB	449	369	0.06%	0.007%
73	11.304	3096	3099	3103	rVB	391	255	0.04%	0.005%
74	11.324	3103	3105	3109	rVB	440	272	0.04%	0.005%
75	11.349	3109	3113	3115	rBV2	525	430	0.07%	0.009%
76	11.459	3144	3147	3150	rBV2	545	446	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
 Data File : VU046299.D
 Acq On : 11 Dec 2021 19:57
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK009

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.574	3177	3183	3185	rBV2	500	458	0.07%	0.009%
78	11.590	3185	3188	3192	rVV	449	421	0.07%	0.008%
79	11.613	3192	3195	3200	rVB	411	290	0.05%	0.006%
80	11.713	3222	3226	3228	rBV2	392	338	0.05%	0.007%
81	11.812	3245	3257	3275	rVB	291989	461223	72.75%	9.220%
82	12.066	3332	3336	3340	rVB2	355	339	0.05%	0.007%
83	12.089	3340	3343	3346	rBV	378	293	0.05%	0.006%
84	12.195	3364	3376	3395	rVB	312351	492673	77.71%	9.849%
85	12.266	3395	3398	3401	rBV	376	273	0.04%	0.005%
86	12.343	3419	3422	3425	rBV2	371	300	0.05%	0.006%
87	12.430	3446	3449	3451	rBV	360	267	0.04%	0.005%
88	12.616	3504	3507	3510	rBV2	319	272	0.04%	0.005%
89	12.825	3566	3572	3580	rBV2	611	1251	0.20%	0.025%
90	12.857	3580	3582	3586	rVB	414	278	0.04%	0.006%
91	13.433	3757	3761	3764	rBV2	401	379	0.06%	0.008%
92	13.738	3853	3856	3858	rBV	340	267	0.04%	0.005%
93	13.921	3910	3913	3916	rVB	429	261	0.04%	0.005%
94	14.057	3953	3955	3960	rBV	464	361	0.06%	0.007%
95	14.159	3984	3987	3990	rBV	498	343	0.05%	0.007%
96	14.436	4069	4073	4075	rBV	426	356	0.06%	0.007%
97	15.230	4314	4320	4322	rBV2	504	528	0.08%	0.011%
98	15.407	4371	4375	4378	rBV2	774	701	0.11%	0.014%
99	16.236	4630	4633	4638	rBV3	538	537	0.08%	0.011%
100	16.519	4718	4721	4722	rBV	607	363	0.06%	0.007%




Sum of corrected areas: 5002363

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
Data File : VU046299.D
Acq On : 11 Dec 2021 19:57
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK009

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

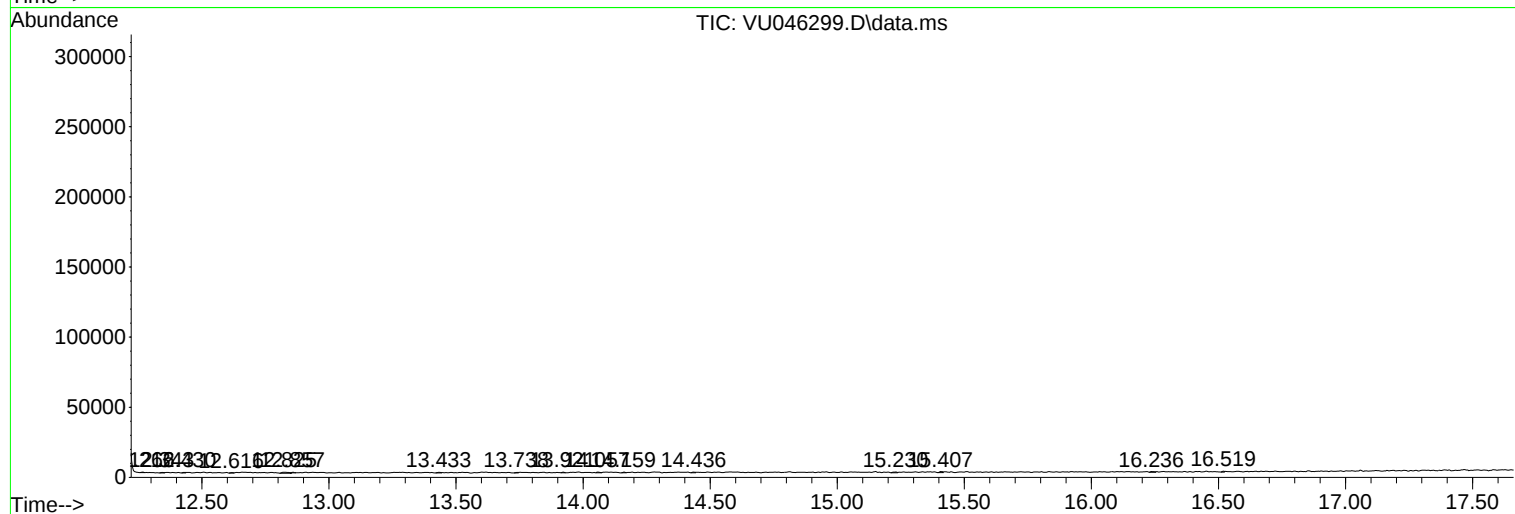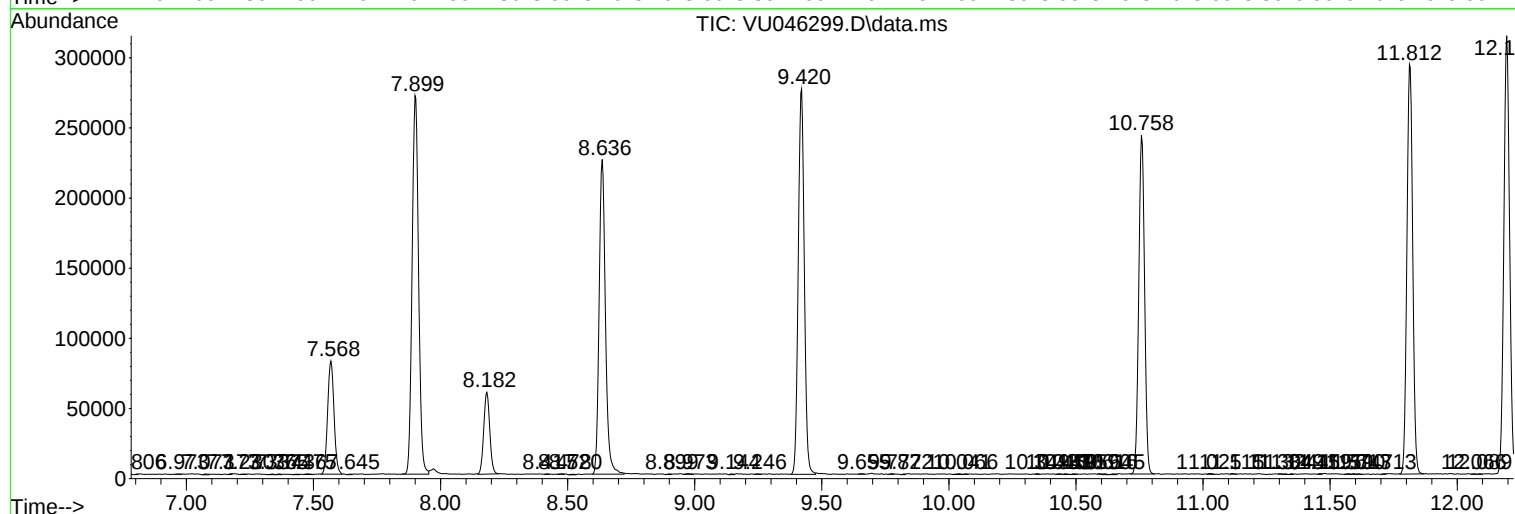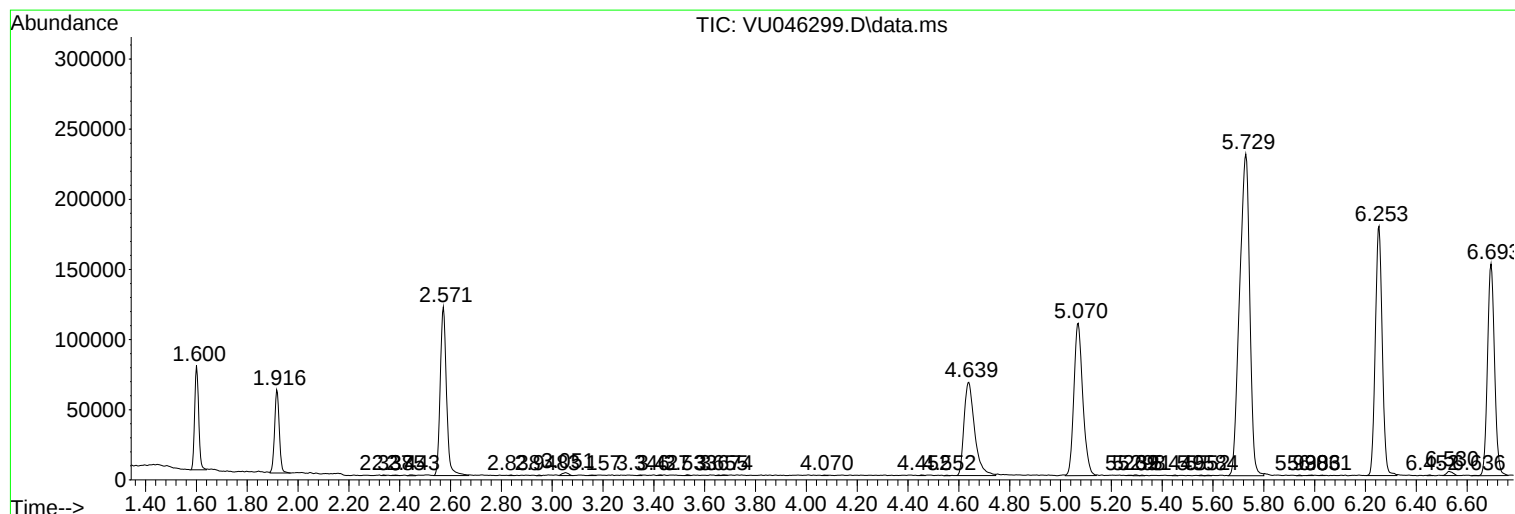

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
Data File : VU046299.D
Acq On : 11 Dec 2021 19:57
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK009

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
Data File : VU046299.D
Acq On : 11 Dec 2021 19:57
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK009

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc