
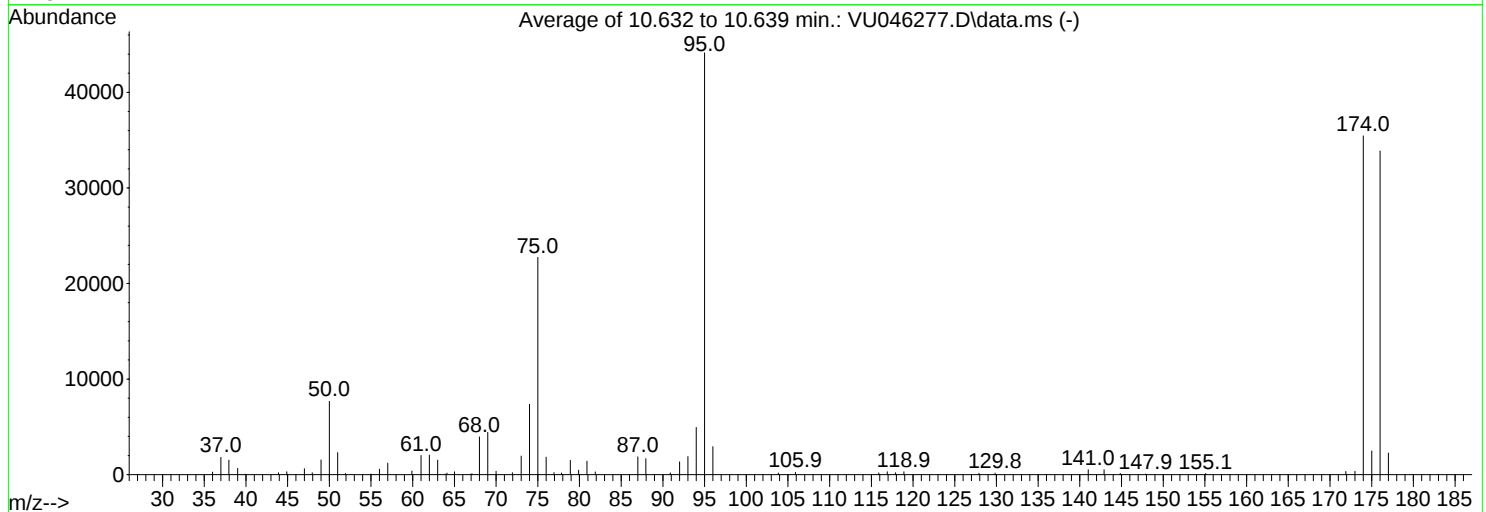


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121121\
 Data File : VU046277.D
 Acq On : 11 Dec 2021 10:54
 Operator : SY/MD
 Sample : BFB029
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB029

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis
 Last Update : Mon Dec 20 00:25:10 2021

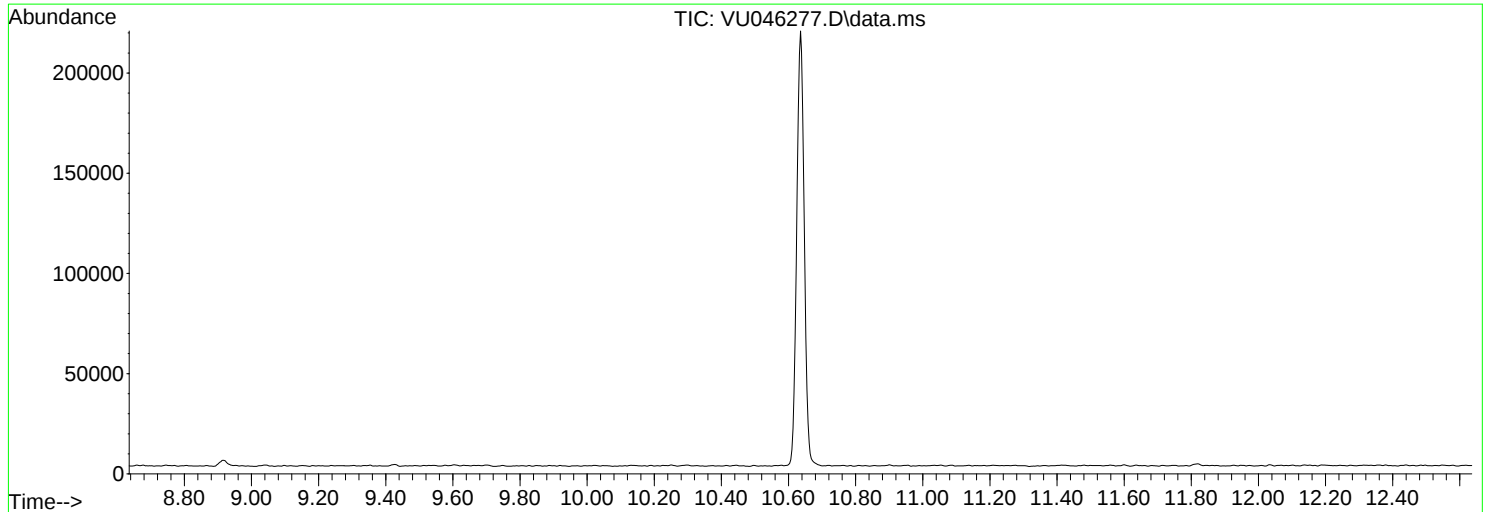

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	7675	PASS
75	95	30	80	51.5	22733	PASS
95	95	100	100	100.0	44136	PASS
96	95	5	9	6.6	2924	PASS
173	174	0.00	2	1.0	346	PASS
174	95	50	120	80.3	35448	PASS
175	174	5	9	7.0	2478	PASS
176	174	95	101	95.6	33875	PASS
177	176	5	9	6.7	2258	PASS

m/z	Abundance
39.90	3977.0
43.90	277.0

Instrument :
MSVOA_U
ClientSampleId :
BFB029

m/z	Abundance
36.00	263.0
37.00	1791.0
37.90	1528.0
39.00	645.0
39.90	3970.0
44.00	485.0
44.90	307.0
47.00	592.0
47.90	207.0
49.00	1538.0
50.00	7610.0
51.00	2251.0
52.00	130.0
56.00	526.0
57.00	1210.0
59.90	407.0
61.00	2065.0
62.00	1932.0
63.00	1493.0
63.90	221.0
65.00	293.0
66.90	139.0
68.00	3974.0
69.00	4303.0
70.00	339.0
72.00	188.0
73.00	2022.0
74.00	7439.0
75.00	22368.0
76.00	1862.0
77.00	230.0
77.80	174.0
78.90	1453.0
79.90	430.0
80.90	1389.0
81.90	299.0
87.00	1932.0
88.00	1648.0
90.90	186.0
92.00	1356.0
93.00	1905.0
94.00	4801.0
95.00	43320.0
96.00	2961.0
103.80	153.0
105.90	214.0
115.90	192.0
116.90	300.0
117.90	192.0
118.90	327.0
127.90	164.0
129.90	154.0
141.00	542.0
142.90	542.0
144.80	119.0
155.10	111.0
171.90	359.0
173.00	322.0
174.00	34312.0
175.00	2457.0
176.00	32552.0
177.00	2131.0

Instrument :
MSVOA_U
ClientSampleId :
BFB029

m/z	Abundance
36.00	274.0
37.00	1893.0
37.90	1593.0
39.00	668.0
39.90	4059.0
43.90	481.0
44.90	315.0
47.00	658.0
47.90	196.0
49.00	1604.0
50.00	7933.0
51.00	2399.0
52.00	132.0
55.00	105.0
56.00	593.0
57.00	1257.0
59.90	400.0
61.00	2037.0
62.00	2091.0
63.00	1549.0
64.10	246.0
65.00	313.0
67.10	141.0
68.00	4037.0
69.00	4578.0
70.00	381.0
71.90	198.0
73.00	1981.0
74.00	7590.0
75.00	23544.0
76.00	1895.0
76.90	225.0
77.90	183.0
78.90	1561.0
79.90	494.0
80.90	1436.0
81.90	288.0
87.00	1921.0
88.00	1700.0
90.90	204.0
92.00	1408.0
93.00	1975.0
94.00	5073.0
95.00	45792.0
96.00	3024.0
103.90	164.0
105.90	256.0
115.90	188.0
116.90	315.0
117.90	230.0
118.90	329.0
127.90	152.0
129.80	177.0
141.00	539.0
142.90	534.0
144.90	132.0
147.90	108.0
155.10	114.0
171.90	345.0
173.00	353.0
174.00	36688.0
175.00	2572.0
176.00	34952.0
177.00	2363.0

Instrument :
MSVOA_U
ClientSampleId :
BFB029

m/z	Abundance
36.00	250.0
37.00	1748.0
38.00	1478.0
39.00	643.0
39.90	4076.0
43.90	462.0
44.90	308.0
47.00	592.0
48.00	202.0
49.00	1481.0
50.00	7481.0
51.00	2302.0
51.90	111.0
55.00	107.0
56.00	577.0
57.00	1145.0
59.90	340.0
61.00	1906.0
62.00	2104.0
63.00	1536.0
64.10	272.0
65.00	292.0
67.10	140.0
68.00	3844.0
69.00	4405.0
70.00	359.0
71.90	196.0
73.00	1821.0
74.00	7053.0
75.00	22288.0
76.00	1740.0
76.90	197.0
77.90	166.0
78.90	1481.0
79.90	461.0
80.90	1381.0
81.90	285.0
87.00	1747.0
87.90	1657.0
90.90	182.0
92.00	1263.0
93.00	1779.0
94.00	4943.0
95.00	43296.0
96.00	2788.0
103.90	163.0
105.90	240.0
115.90	160.0
116.90	292.0
117.90	203.0
118.90	274.0
127.90	154.0
129.80	185.0
141.00	493.0
142.90	474.0
144.90	148.0
147.90	100.0
155.10	116.0
171.90	288.0
173.00	363.0
174.00	35344.0
175.00	2404.0
176.00	34120.0
177.00	2280.0

Instrument :
MSVOA_U
ClientSampleId :
BFB029