

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121124\
 Data File : VU062244.D
 Acq On : 11 Dec 2024 16:33
 Operator : MD/SY
 Sample : P5253-01
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7J51

Quant Time: Dec 12 00:28:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 12 00:24:05 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	105920	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	102115	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	47512	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	24305	3.402	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.000%
7) Chloroethane-d5	1.908	69	20521	4.038	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	80.800%
11) 1,1-Dichloroethene-d2	2.557	65	12462	3.667	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.400%
20) 2-Butanone-d5	4.628	46	62449	45.609	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.220%
24) Chloroform-d	5.052	84	65259	4.221	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.400%
26) 1,2-Dichloroethane-d4	5.692	65	35761	4.703	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.000%
32) Benzene-d6	5.718	84	118096	4.015	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.400%
36) 1,2-Dichloropropane-d6	6.682	67	35826	4.257	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.200%
41) Toluene-d8	7.891	98	105838	3.809	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.200%
43) trans-1,3-Dichloroprop...	8.174	79	15148	4.090	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.800%
46) 2-Hexanone-d5	8.628	63	46641	41.738	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.480%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	28779	4.395	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.000%
66) 1,2-Dichlorobenzene-d4	12.187	152	39911	4.558	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.200%
Target Compounds					Qvalue	
13) Acetone	2.647	43	6277	6.733	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121124\
Data File : VU062244.D
Acq On : 11 Dec 2024 16:33
Operator : MD/SY
Sample : P5253-01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7J51

Quant Time: Dec 12 00:28:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 12 00:24:05 2024
Response via : Initial Calibration

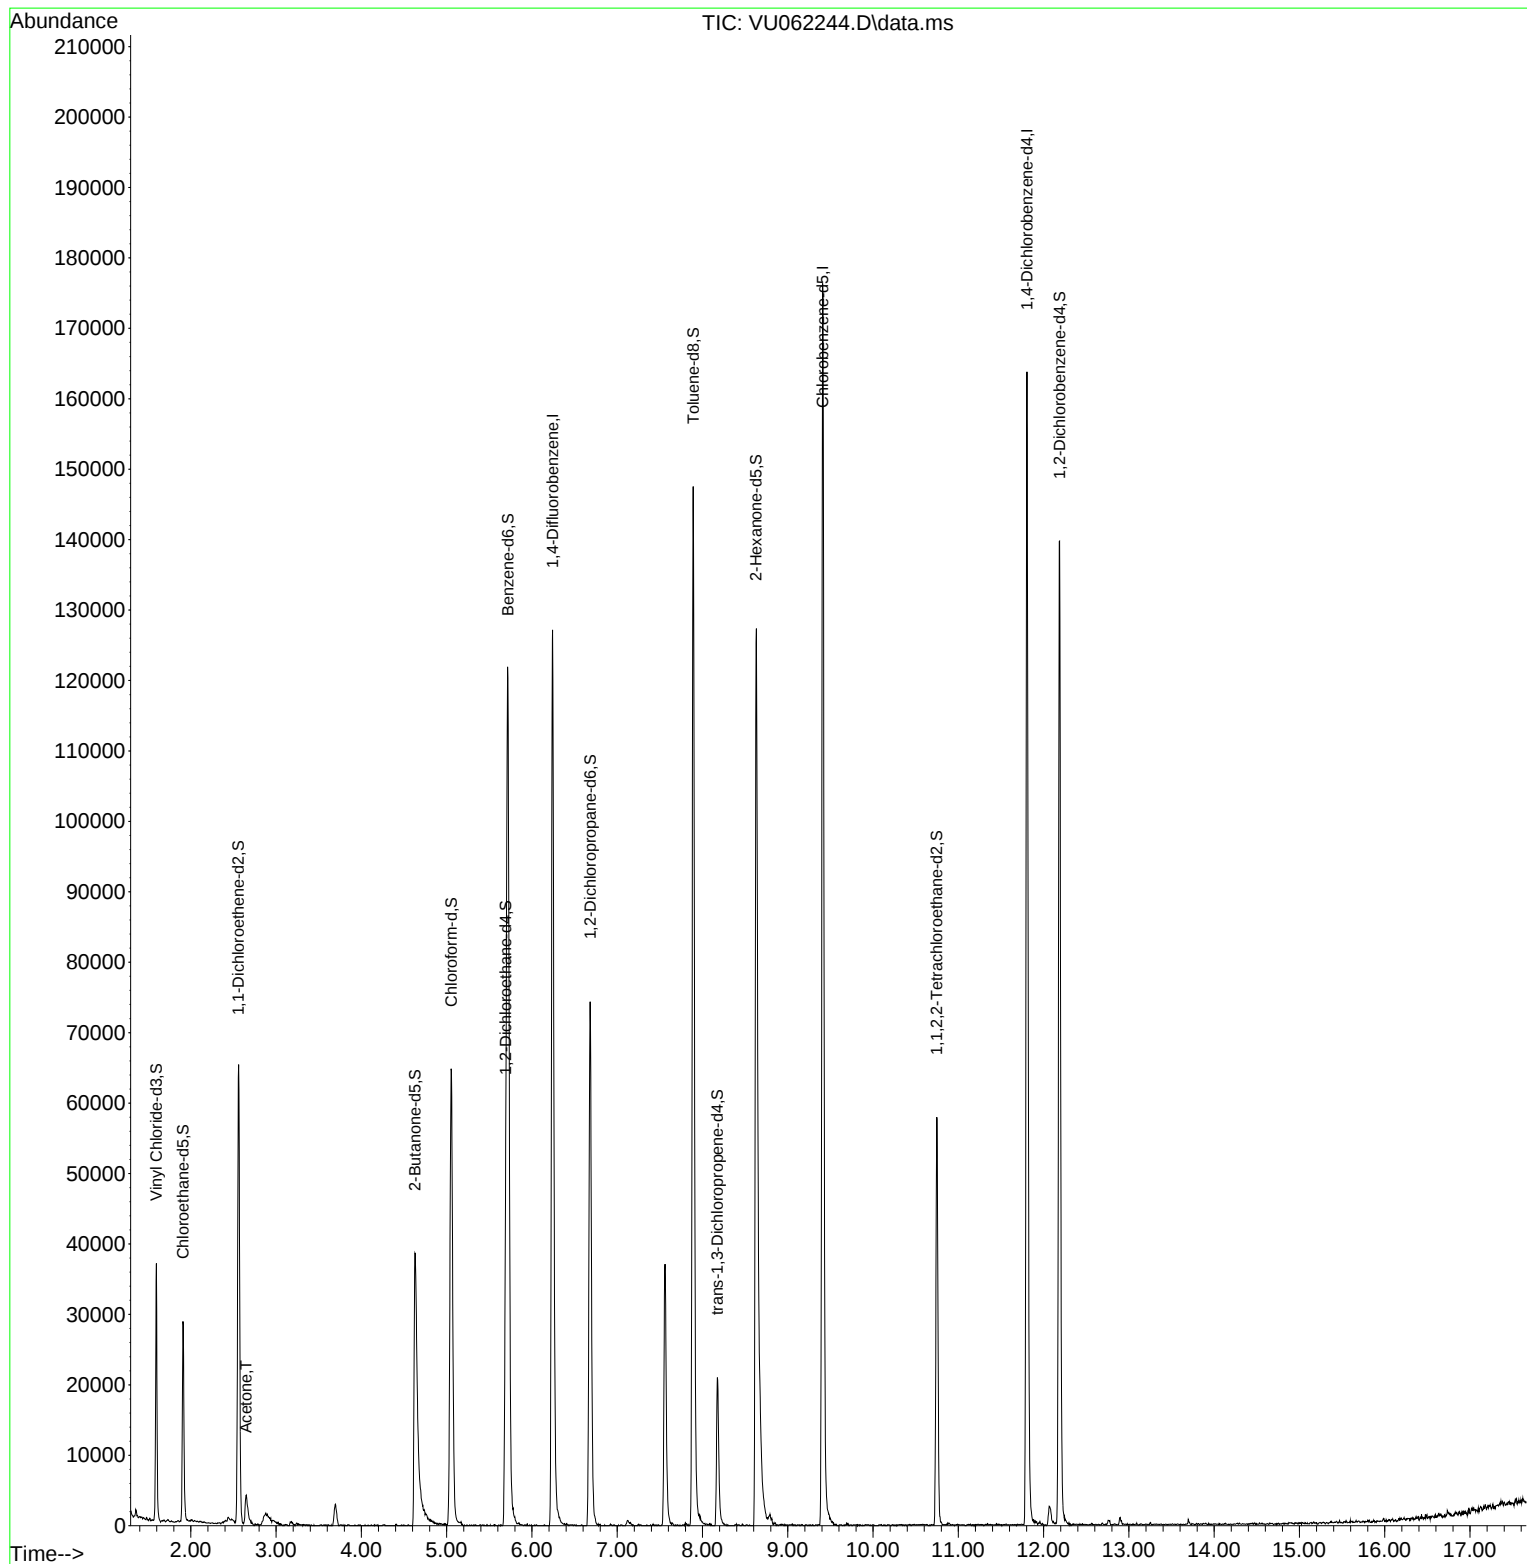

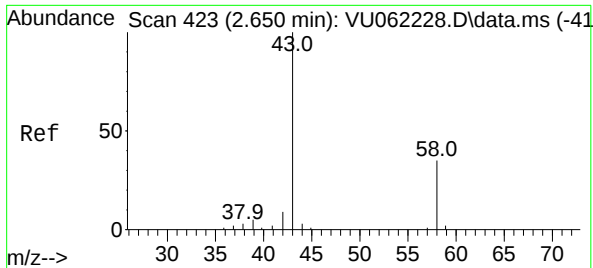

#13
 Acetone
 Concen: 6.733 ug/L
 RT: 2.647 min Scan# 41
 Delta R.T. -0.003 min
 Lab File: VU062244.D
 Acq: 11 Dec 2024 16:33

Instrument :
 MSVOA_U
 ClientSampleId :
 F7J51

Tgt Ion: 43 Resp: 6277
 Ion Ratio Lower Upper
 43 100
 58 32.5 0.0 64.0

