

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121124\
 Data File : VU062245.D
 Acq On : 11 Dec 2024 16:58
 Operator : MD/SY
 Sample : P5253-02
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7J53

Quant Time: Dec 12 00:29:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 12 00:24:05 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	96641	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	91791	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	42970	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	23944	3.673	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.400%
7) Chloroethane-d5	1.911	69	19391	4.182	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.600%
11) 1,1-Dichloroethene-d2	2.560	65	12078	3.895	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.800%
20) 2-Butanone-d5	4.631	46	61355	49.113	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.220%
24) Chloroform-d	5.052	84	64453	4.569	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.400%
26) 1,2-Dichloroethane-d4	5.695	65	34314	4.946	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.000%
32) Benzene-d6	5.717	84	114047	4.314	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.200%
36) 1,2-Dichloropropane-d6	6.682	67	35056	4.634	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.600%
41) Toluene-d8	7.891	98	102082	4.087	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.800%
43) trans-1,3-Dichloroprop...	8.174	79	14355	4.311	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.200%
46) 2-Hexanone-d5	8.627	63	46531	46.323	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.640%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	28022	4.761	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.200%
66) 1,2-Dichlorobenzene-d4	12.187	152	38901	4.913	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.200%
Target Compounds						
13) Acetone	2.653	43	10238	12.036	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121124\
Data File : VU062245.D
Acq On : 11 Dec 2024 16:58
Operator : MD/SY
Sample : P5253-02
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7J53

Quant Time: Dec 12 00:29:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 12 00:24:05 2024
Response via : Initial Calibration

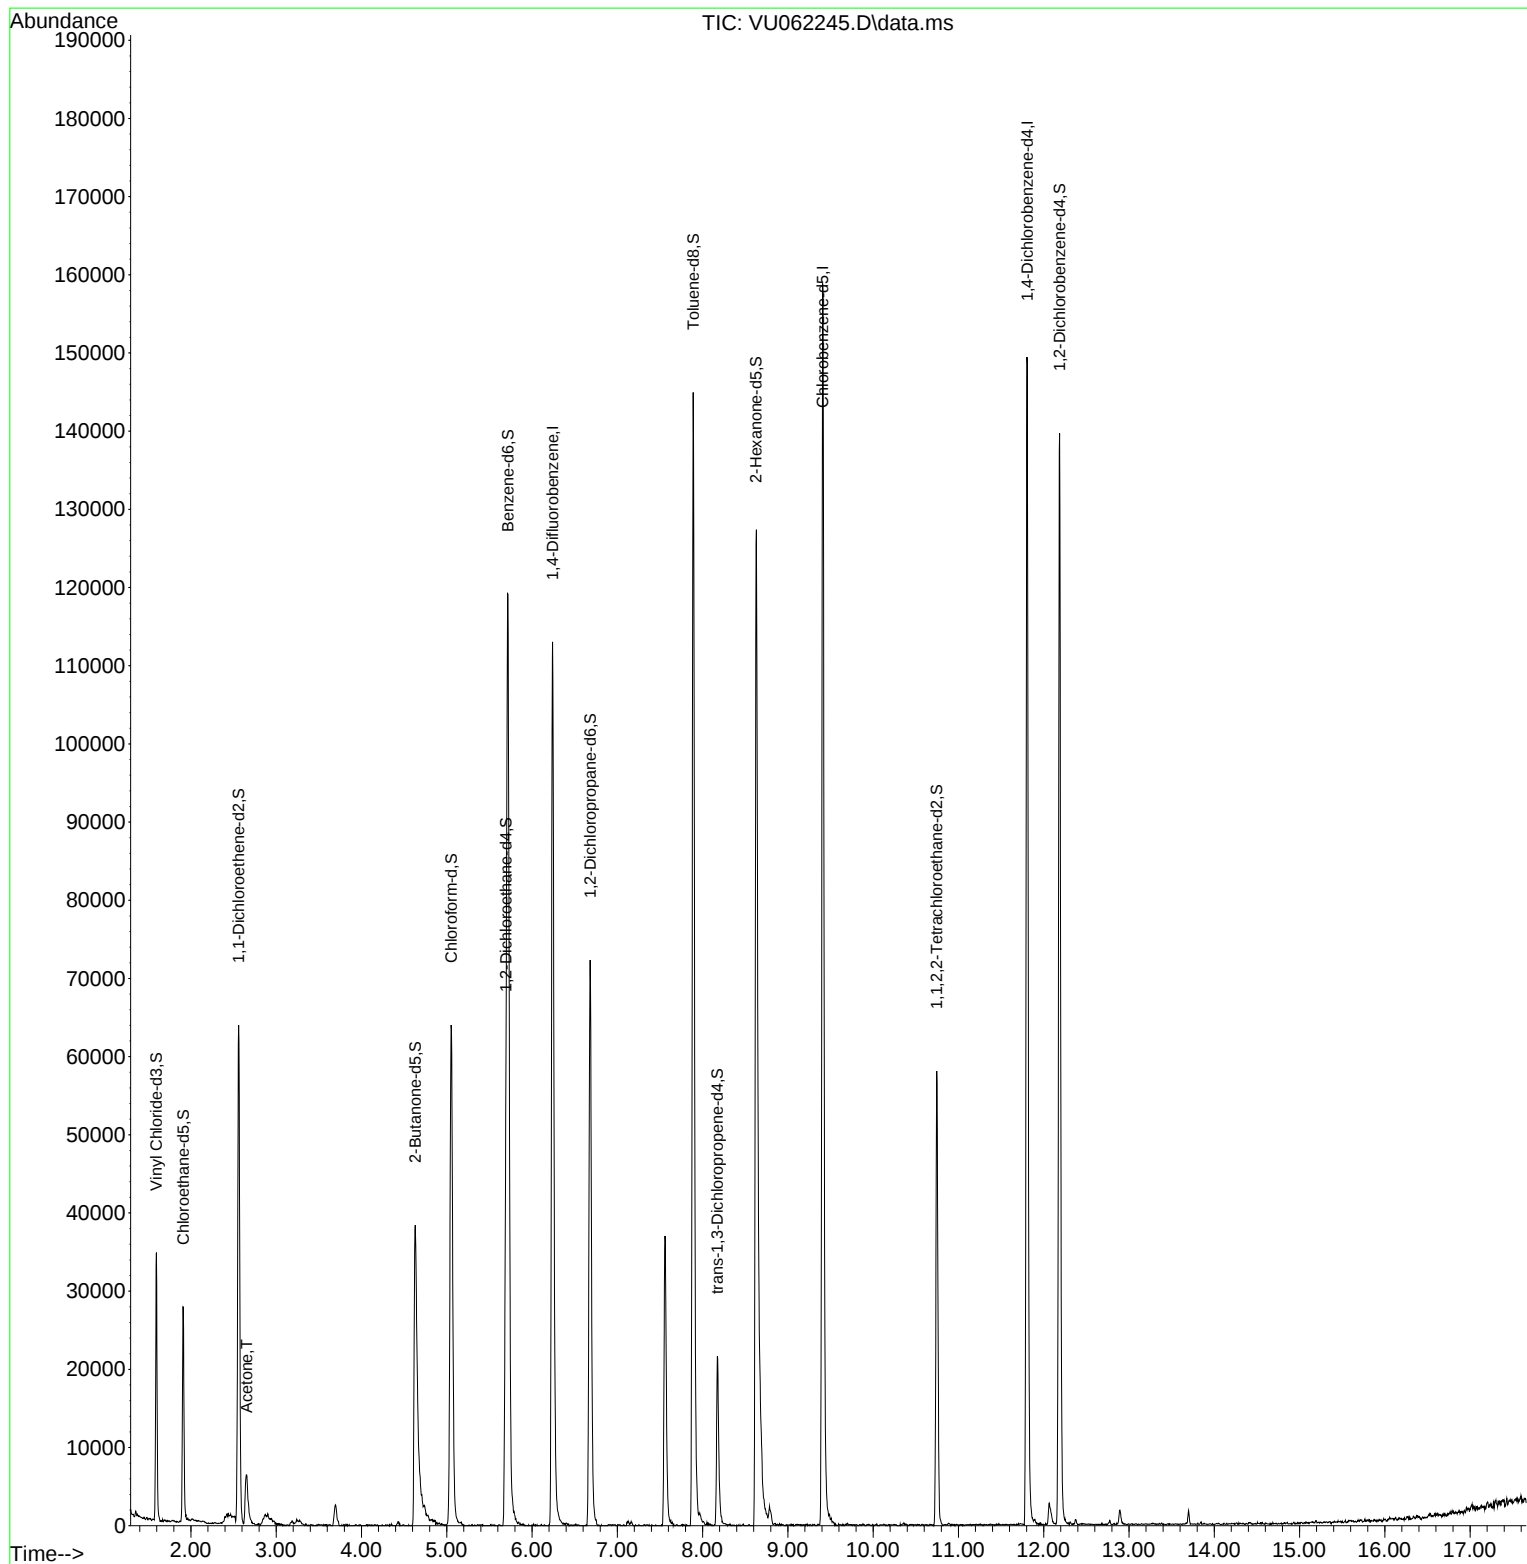

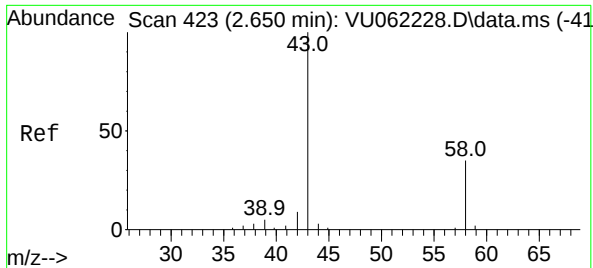

#13
 Acetone
 Concen: 12.036 ug/L
 RT: 2.653 min Scan# 41
 Delta R.T. 0.003 min
 Lab File: VU062245.D
 Acq: 11 Dec 2024 16:58

Instrument :
 MSVOA_U
 ClientSampleId :
 F7J53

Tgt Ion: 43 Resp: 10238
 Ion Ratio Lower Upper
 43 100
 58 34.9 0.0 64.0

