

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121124\
 Data File : VU062246.D
 Acq On : 11 Dec 2024 17:22
 Operator : MD/SY
 Sample : P5253-03
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7J54

Quant Time: Dec 12 00:29:28 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 12 00:24:05 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	97675	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	88835	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	41473	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	24452	3.711	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.200%
7) Chloroethane-d5	1.911	69	19640	4.191	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.800%
11) 1,1-Dichloroethene-d2	2.560	65	12758	4.070	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.400%
20) 2-Butanone-d5	4.631	46	65843	52.147	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.300%
24) Chloroform-d	5.052	84	65362	4.584	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.600%
26) 1,2-Dichloroethane-d4	5.695	65	35354	5.042	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.800%
32) Benzene-d6	5.717	84	114251	4.465	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.400%
36) 1,2-Dichloropropane-d6	6.682	67	34756	4.748	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.000%
41) Toluene-d8	7.891	98	102910	4.258	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.200%
43) trans-1,3-Dichloroprop...	8.177	79	14703	4.563	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.200%
46) 2-Hexanone-d5	8.627	63	48797	50.195	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.400%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	28765	5.050	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.000%
66) 1,2-Dichlorobenzene-d4	12.187	152	38548	5.044	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.800%
Target Compounds						Qvalue
13) Acetone	2.647	43	11757	13.676	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121124\
Data File : VU062246.D
Acq On : 11 Dec 2024 17:22
Operator : MD/SY
Sample : P5253-03
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7J54

Quant Time: Dec 12 00:29:28 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 12 00:24:05 2024
Response via : Initial Calibration

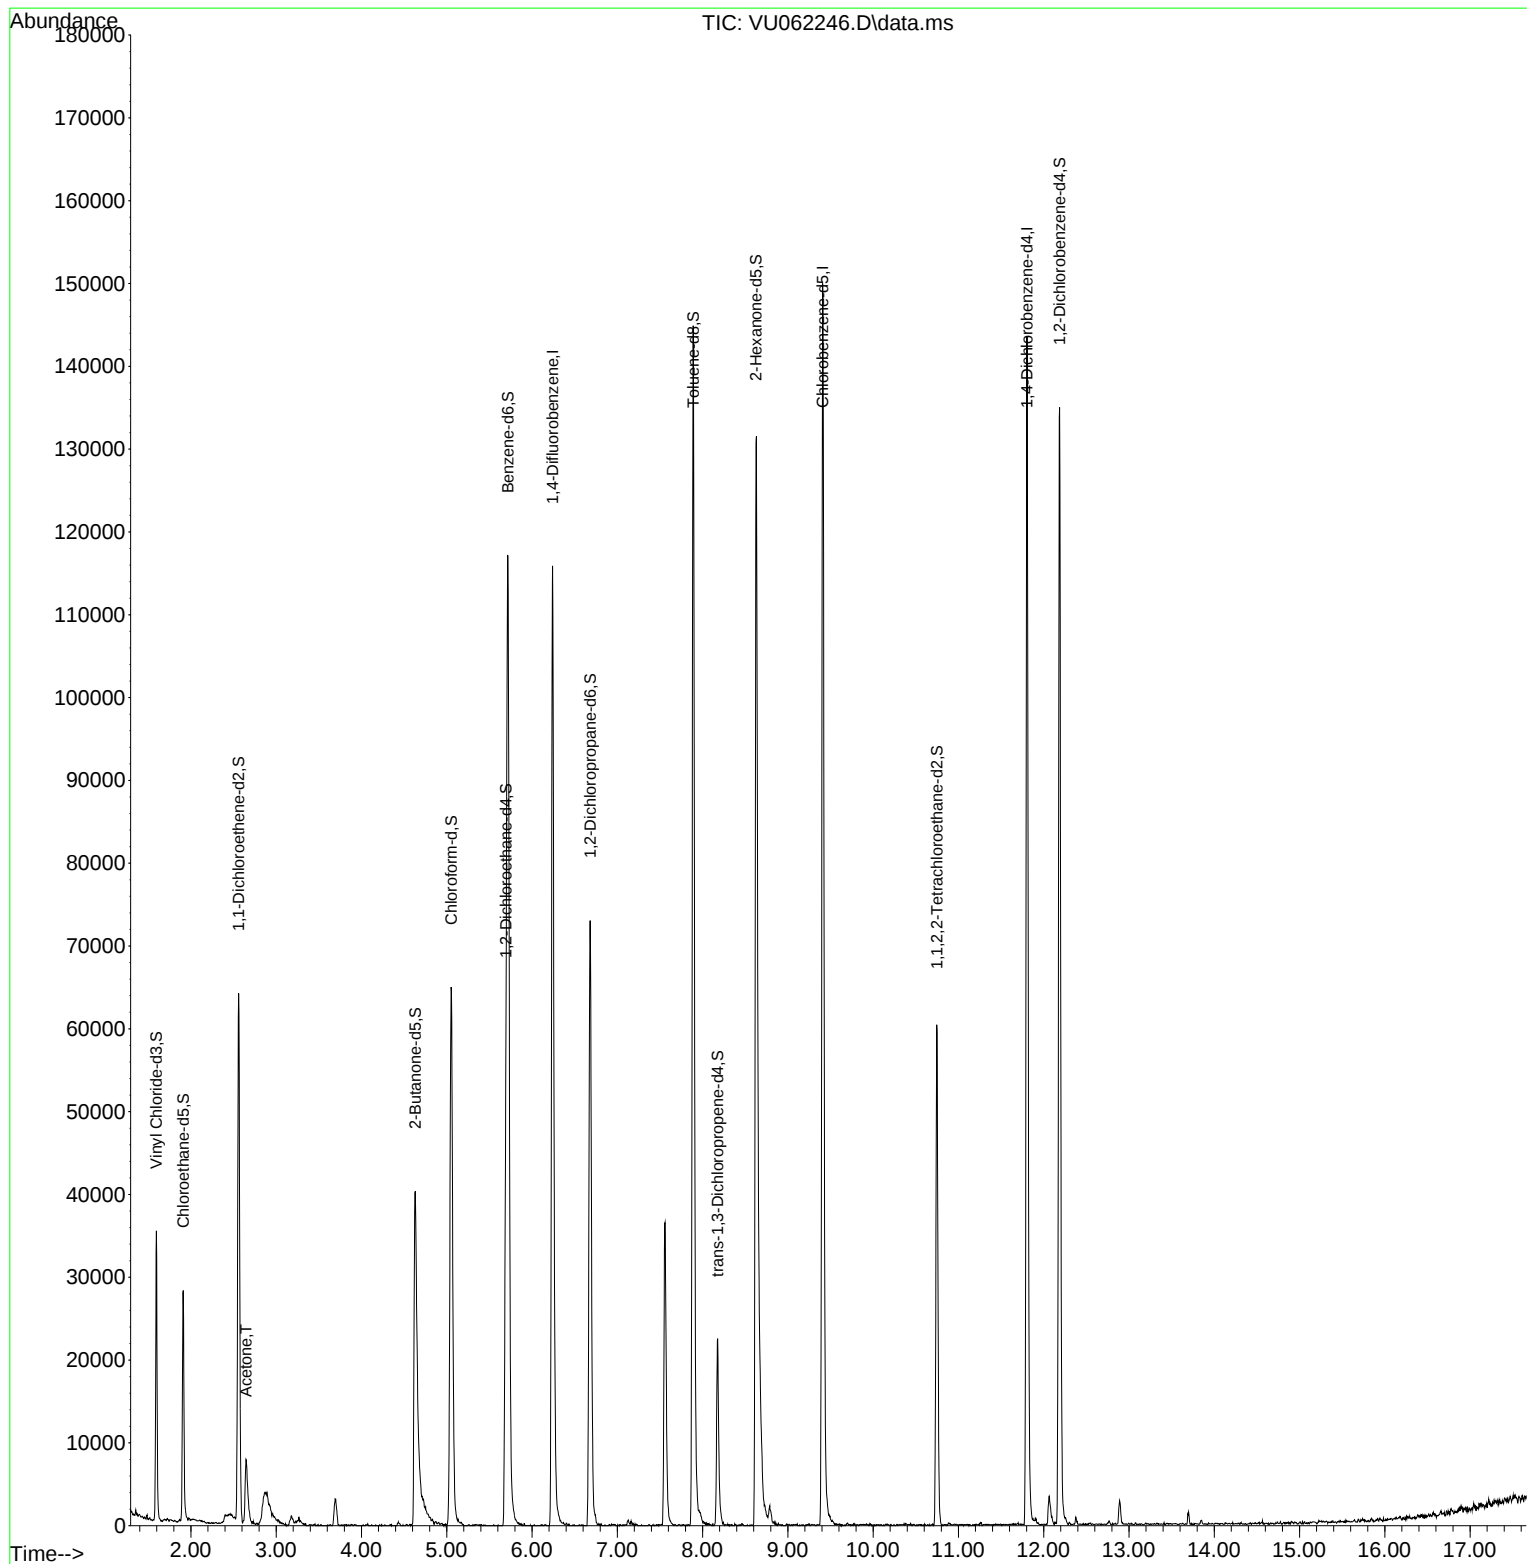

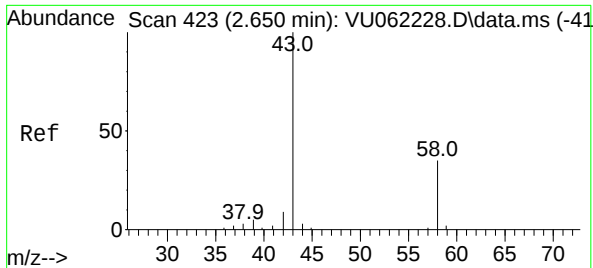

Acetone
 Concen: 13.676 ug/L
 RT: 2.647 min Scan# 41
 Delta R.T. -0.003 min
 Lab File: VU062246.D
 Acq: 11 Dec 2024 17:22

Instrument :
 MSVOA_U
 ClientSampleId :
 F7J54

Tgt Ion: 43	Resp: 11757
Ion Ratio	Lower Upper
43	100
58	34.7 0.0 64.0

