
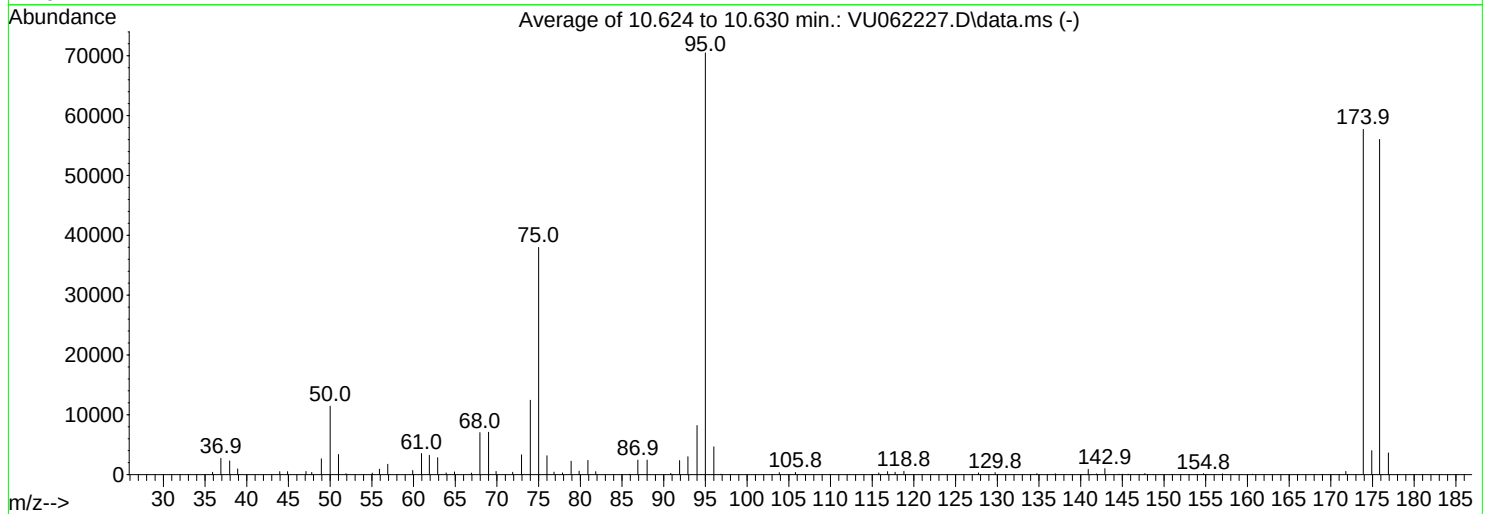


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121124\
Data File : VU062227.D
Acq On : 11 Dec 2024 08:56
Operator : MD/SY
Sample : BFB044
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB044

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Dec 13 00:13:55 2024

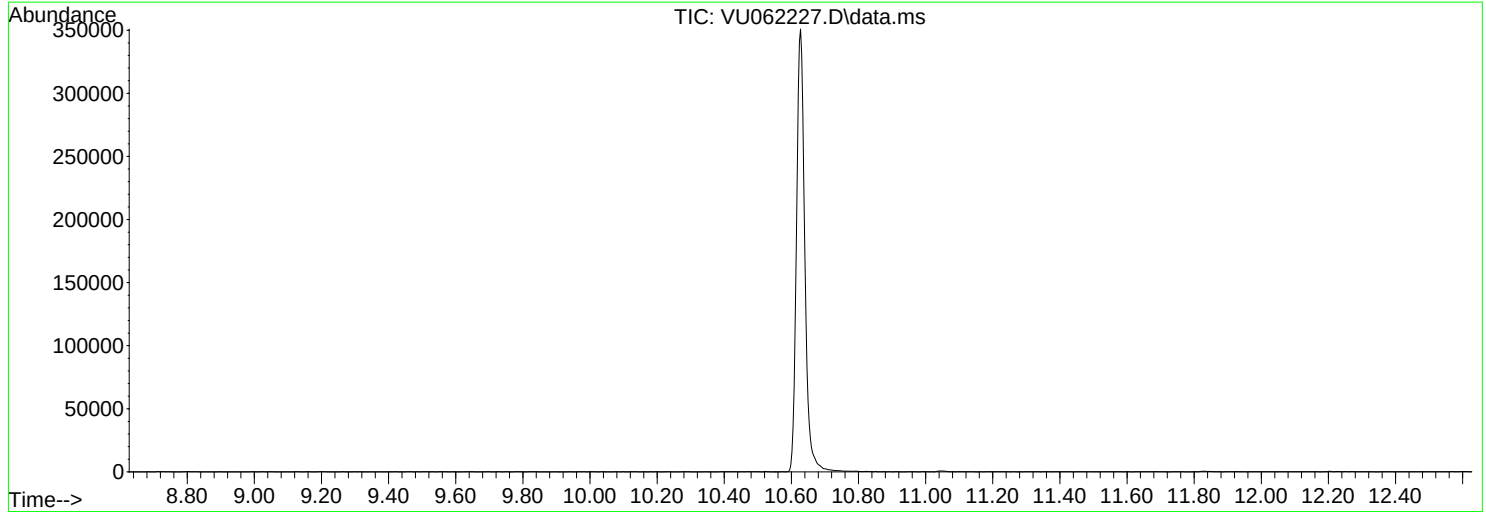

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.2	11445	PASS
75	95	30	80	53.9	37987	PASS
95	95	100	100	100.0	70493	PASS
96	95	5	9	6.6	4656	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	81.9	57715	PASS
175	174	5	9	7.0	4023	PASS
176	174	95	101	97.1	56024	PASS
177	176	5	9	6.5	3631	PASS

m/z Abundance

Instrument :
MSVOA_U
ClientSampleId :
BFB044

m/z	Abundance
35.90	383.0
36.90	2860.0
38.00	2410.0
38.90	985.0
43.90	564.0
44.90	532.0
47.10	563.0
47.80	348.0
48.90	2641.0
50.00	11325.0
51.00	3447.0
51.90	192.0
55.00	223.0
55.90	939.0
56.90	1671.0
59.90	891.0
61.00	3572.0
61.90	3261.0
62.90	2760.0
63.90	349.0
64.90	453.0
67.00	251.0
67.90	7211.0
69.00	7114.0
69.90	577.0
71.90	380.0
73.00	3490.0
74.00	12487.0
75.00	38872.0
76.00	3141.0
76.80	437.0
77.90	303.0
78.90	2238.0
79.90	610.0
80.90	2416.0
81.90	488.0
86.90	2497.0
88.00	2515.0
90.90	225.0
91.90	2515.0
92.90	2976.0
94.00	8356.0
95.00	70696.0
96.00	4779.0
103.80	327.0
105.80	371.0
115.80	302.0
116.90	535.0
117.70	391.0
118.80	582.0
127.70	328.0
128.70	123.0
129.80	318.0
134.80	188.0
137.00	164.0
140.90	883.0
141.90	105.0
142.90	1005.0
144.60	110.0
147.70	185.0
154.80	171.0
157.00	108.0
160.60	123.0
171.90	498.0
173.90	57024.0
174.90	3953.0
175.80	54688.0
176.90	3608.0

Instrument :
MSVOA_U
ClientSampleId :
BFB044

m/z	Abundance
35.90	393.0
36.90	2844.0
38.00	2325.0
38.90	975.0
44.00	548.0
44.90	513.0
47.10	566.0
47.80	397.0
49.00	2695.0
50.00	11826.0
51.00	3430.0
51.90	196.0
55.10	267.0
55.90	914.0
56.90	1767.0
59.90	692.0
61.00	3646.0
61.90	3309.0
62.90	2948.0
63.90	300.0
64.90	455.0
67.00	234.0
67.90	7274.0
69.00	7246.0
69.90	528.0
71.90	419.0
73.00	3422.0
74.00	12817.0
75.00	39048.0
76.00	3271.0
76.90	459.0
77.90	314.0
78.90	2299.0
79.80	607.0
80.90	2437.0
81.80	515.0
86.90	2545.0
88.00	2519.0
90.80	223.0
91.90	2437.0
92.90	3041.0
94.00	8506.0
95.00	72616.0
96.00	4759.0
96.80	110.0
103.90	348.0
105.80	409.0
106.80	110.0
115.80	321.0
116.80	509.0
117.80	411.0
118.80	594.0
127.70	294.0
129.80	374.0
134.70	186.0
137.00	154.0
140.90	907.0
141.90	146.0
142.90	1029.0
144.60	108.0
145.00	116.0
145.70	118.0
147.70	209.0
154.70	175.0
157.00	153.0
160.60	103.0
171.80	513.0
173.90	59360.0
174.90	4148.0
175.80	57712.0
176.90	3774.0

Instrument :
MSVOA_U
ClientSampleId :
BFB044

m/z	Abundance
35.90	420.0
36.90	2511.0
37.90	2192.0
38.90	907.0
44.00	452.0
44.90	457.0
47.10	506.0
47.80	411.0
48.90	2572.0
50.00	11183.0
51.00	3213.0
51.90	136.0
55.00	280.0
55.90	878.0
56.90	1783.0
59.90	487.0
60.90	3346.0
61.90	3127.0
62.90	2766.0
63.90	256.0
64.90	431.0
66.80	183.0
67.00	181.0
68.00	6627.0
69.00	6882.0
69.90	475.0
71.90	412.0
72.90	3017.0
74.00	12044.0
75.00	36040.0
76.00	3054.0
76.90	430.0
77.80	275.0
78.90	2171.0
79.80	588.0
80.90	2280.0
81.80	532.0
85.90	147.0
86.90	2273.0
88.00	2280.0
90.80	225.0
91.90	2100.0
92.90	2955.0
94.00	7769.0
95.00	68168.0
96.00	4431.0
96.90	101.0
103.90	363.0
105.80	351.0
115.80	277.0
116.80	444.0
117.80	418.0
118.80	511.0
127.80	272.0
129.70	362.0
134.70	201.0
136.80	132.0
140.90	880.0
141.90	152.0
142.90	1027.0
145.00	112.0
145.70	127.0
147.70	209.0
148.70	103.0
154.70	187.0
157.00	174.0
171.70	581.0
173.90	56760.0
174.90	3969.0
175.90	55672.0
176.90	3512.0

Instrument :
MSVOA_U
ClientSampleId :
BFB044