

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121224\
 Data File : VU062278.D
 Acq On : 12 Dec 2024 11:12
 Operator : MD/SY
 Sample : P5253-01
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7J51

Quant Time: Dec 13 00:15:18 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Dec 13 00:13:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	92165	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	87027	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	40771	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	23085	3.713	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.200%
7) Chloroethane-d5	1.911	69	19756	4.468	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.400%
11) 1,1-Dichloroethene-d2	2.560	65	11559	3.908	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.200%
20) 2-Butanone-d5	4.631	46	60869	51.090	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.180%
24) Chloroform-d	5.055	84	59891	4.451	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.000%
26) 1,2-Dichloroethane-d4	5.692	65	33039	4.994	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.800%
32) Benzene-d6	5.717	84	108480	4.328	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.600%
36) 1,2-Dichloropropane-d6	6.682	67	33105	4.616	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.400%
41) Toluene-d8	7.891	98	97422	4.114	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.200%
43) trans-1,3-Dichloroprop...	8.174	79	13577	4.301	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.000%
46) 2-Hexanone-d5	8.627	63	49350	51.819	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.640%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	27035	4.844	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.800%
66) 1,2-Dichlorobenzene-d4	12.187	152	36481	4.856	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.200%
Target Compounds						
					Qvalue	
13) Acetone	2.650	43	5745	7.082	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121224\
Data File : VU062278.D
Acq On : 12 Dec 2024 11:12
Operator : MD/SY
Sample : P5253-01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7J51


Quant Time: Dec 13 00:15:18 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Dec 13 00:13:55 2024
Response via : Initial Calibration

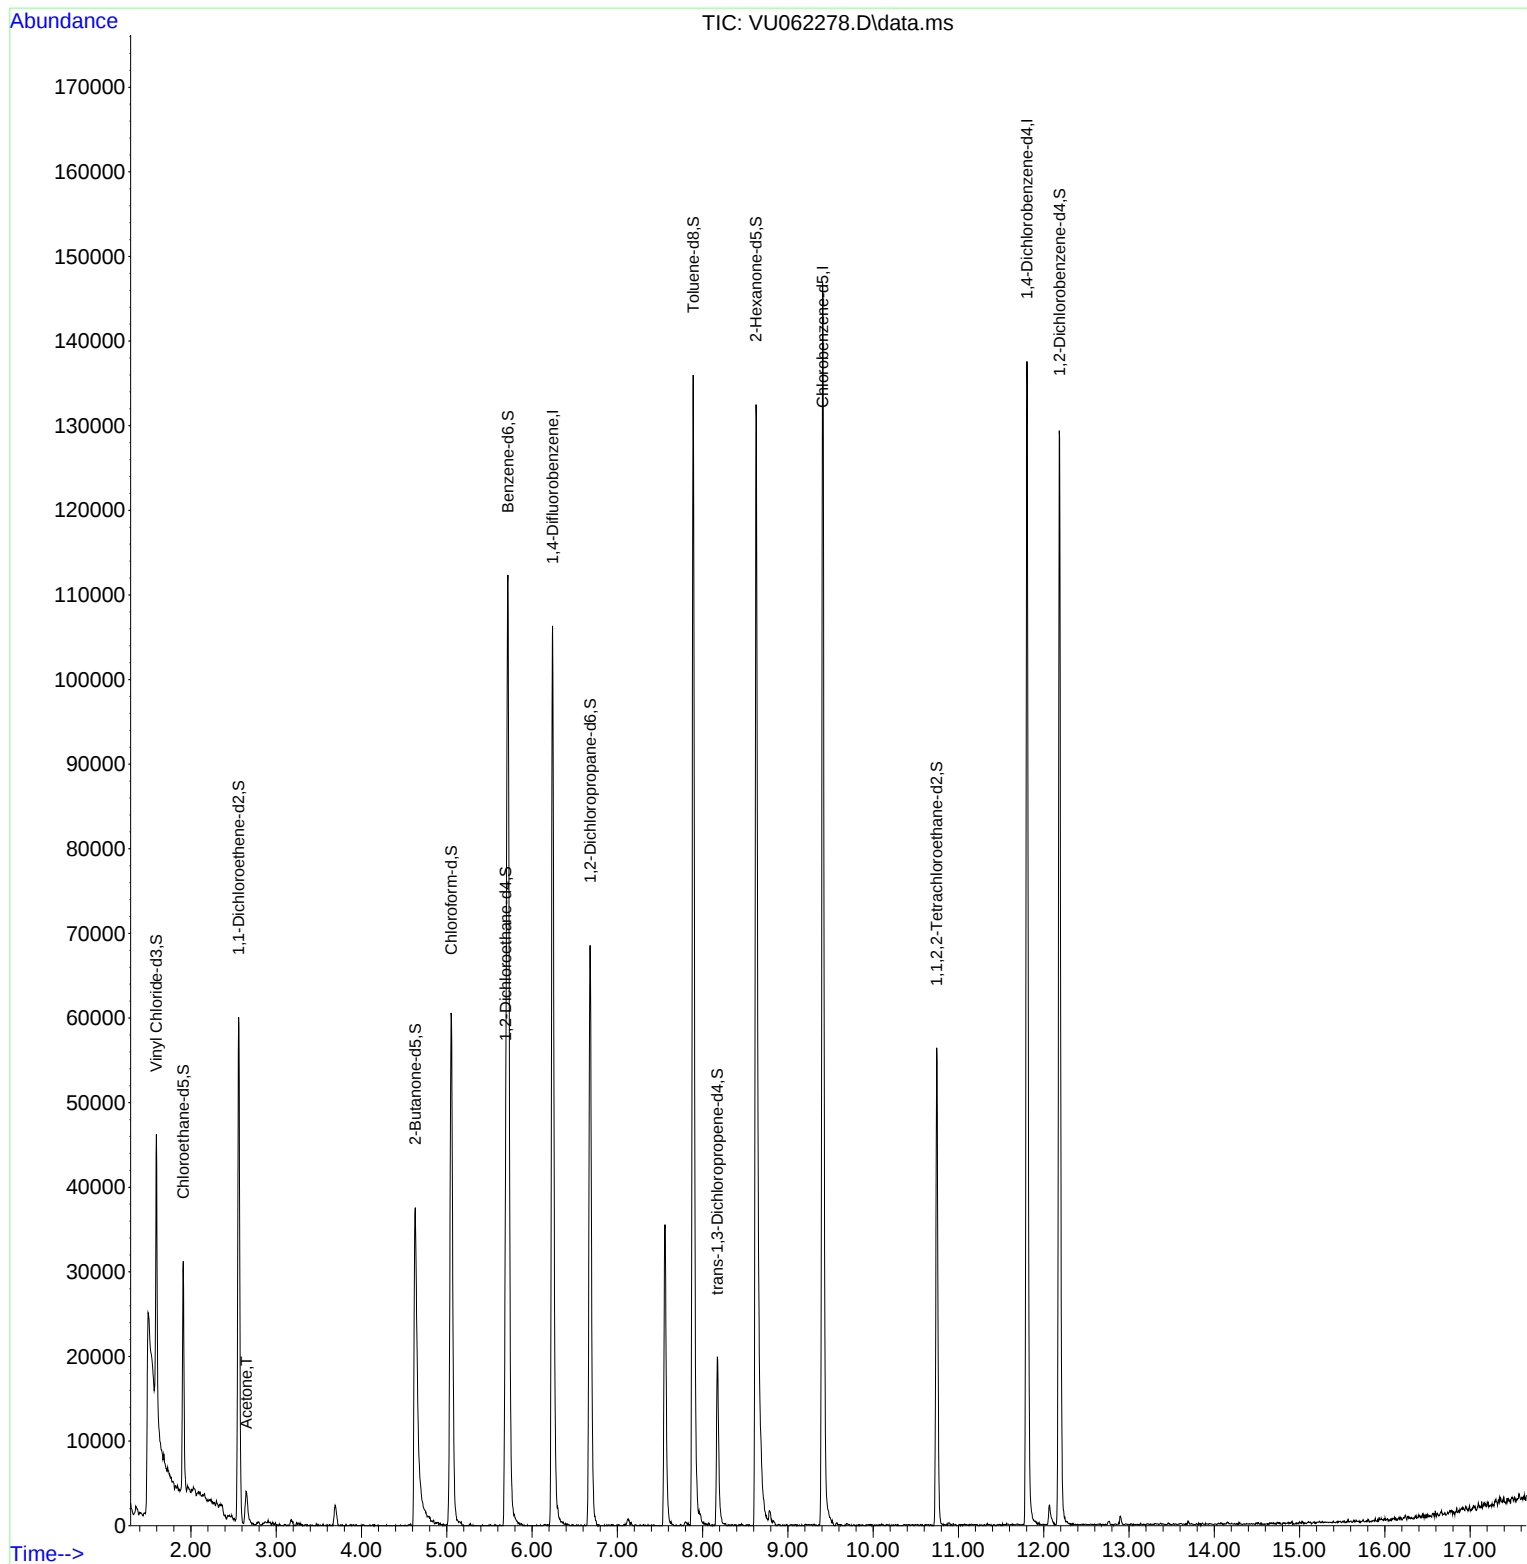

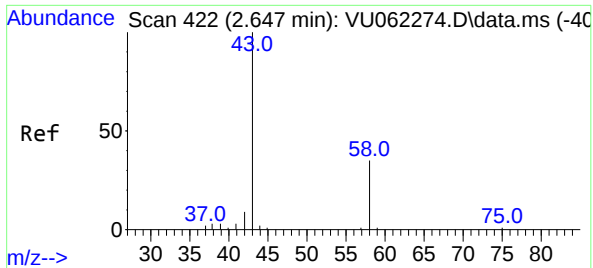

#13
Acetone
Concen: 7.082 ug/L
RT: 2.650 min Scan# 41
Delta R.T. 0.003 min
Lab File: VU062278.D
Acq: 12 Dec 2024 11:12

Instrument :
MSVOA_U
ClientSampleId :
F7J51

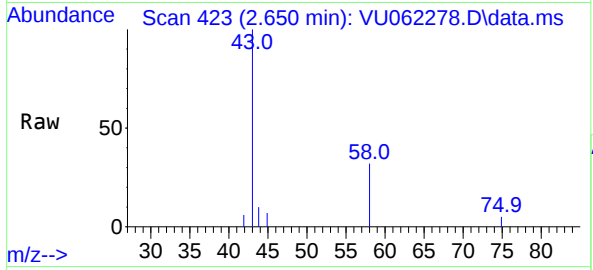

Tgt Ion: 43 Resp: 5745
Ion Ratio Lower Upper
43 100
58 30.3 0.0 64.0

