

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU121224\  
 Data File : VU062290.D  
 Acq On : 12 Dec 2024 16:06  
 Operator : MD/SY  
 Sample : P5253-13  
 Misc : 25mL/MSVOA\_U/WATER  
 ALS Vial : 19 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 F7J56

Quant Time: Dec 13 00:18:36 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR120924WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Fri Dec 13 00:13:55 2024  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc     | Units  | Dev(Min) |
|-------------------------------|--------|-------|----------|----------|--------|----------|
| -----                         |        |       |          |          |        |          |
| Internal Standards            |        |       |          |          |        |          |
| 1) 1,4-Difluorobenzene        | 6.242  | 114   | 87925    | 5.000    | ug/L   | 0.00     |
| 28) Chlorobenzene-d5          | 9.409  | 117   | 82804    | 5.000    | ug/L   | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.804 | 152   | 37860    | 5.000    | ug/L   | 0.00     |
| System Monitoring Compounds   |        |       |          |          |        |          |
| 4) Vinyl Chloride-d3          | 1.596  | 65    | 22348    | 3.768    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 40 - 130 | Recovery | =      | 75.400%  |
| 7) Chloroethane-d5            | 1.907  | 69    | 19496    | 4.622    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 130 | Recovery | =      | 92.400%  |
| 11) 1,1-Dichloroethene-d2     | 2.560  | 65    | 11519    | 4.083    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 125 | Recovery | =      | 81.600%  |
| 20) 2-Butanone-d5             | 4.628  | 46    | 63134    | 55.547   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 40 - 130 | Recovery | =      | 111.100% |
| 24) Chloroform-d              | 5.052  | 84    | 60782    | 4.736    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 94.800%  |
| 26) 1,2-Dichloroethane-d4     | 5.692  | 65    | 33744    | 5.346    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 107.000% |
| 32) Benzene-d6                | 5.718  | 84    | 108589   | 4.553    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 91.000%  |
| 36) 1,2-Dichloropropane-d6    | 6.682  | 67    | 33424    | 4.898    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 140 | Recovery | =      | 98.000%  |
| 41) Toluene-d8                | 7.891  | 98    | 96343    | 4.276    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 85.600%  |
| 43) trans-1,3-Dichloroprop... | 8.174  | 79    | 13328    | 4.437    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 55 - 130 | Recovery | =      | 88.800%  |
| 46) 2-Hexanone-d5             | 8.627  | 63    | 46886    | 51.742   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 45 - 130 | Recovery | =      | 103.480% |
| 56) 1,1,2,2-Tetrachloroeth... | 10.746 | 84    | 27914    | 5.257    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 120 | Recovery | =      | 105.200% |
| 66) 1,2-Dichlorobenzene-d4    | 12.184 | 152   | 36647    | 5.253    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 80 - 120 | Recovery | =      | 105.000% |
| Target Compounds              |        |       |          |          |        |          |
|                               |        |       |          |          | Qvalue |          |
| 13) Acetone                   | 2.647  | 43    | 10323    | 13.339   | ug/L   | 97       |
| -----                         |        |       |          |          |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU121224\  
Data File : VU062290.D  
Acq On : 12 Dec 2024 16:06  
Operator : MD/SY  
Sample : P5253-13  
Misc : 25mL/MSVOA\_U/WATER  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
F7J56

Quant Time: Dec 13 00:18:36 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR120924WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Fri Dec 13 00:13:55 2024  
Response via : Initial Calibration

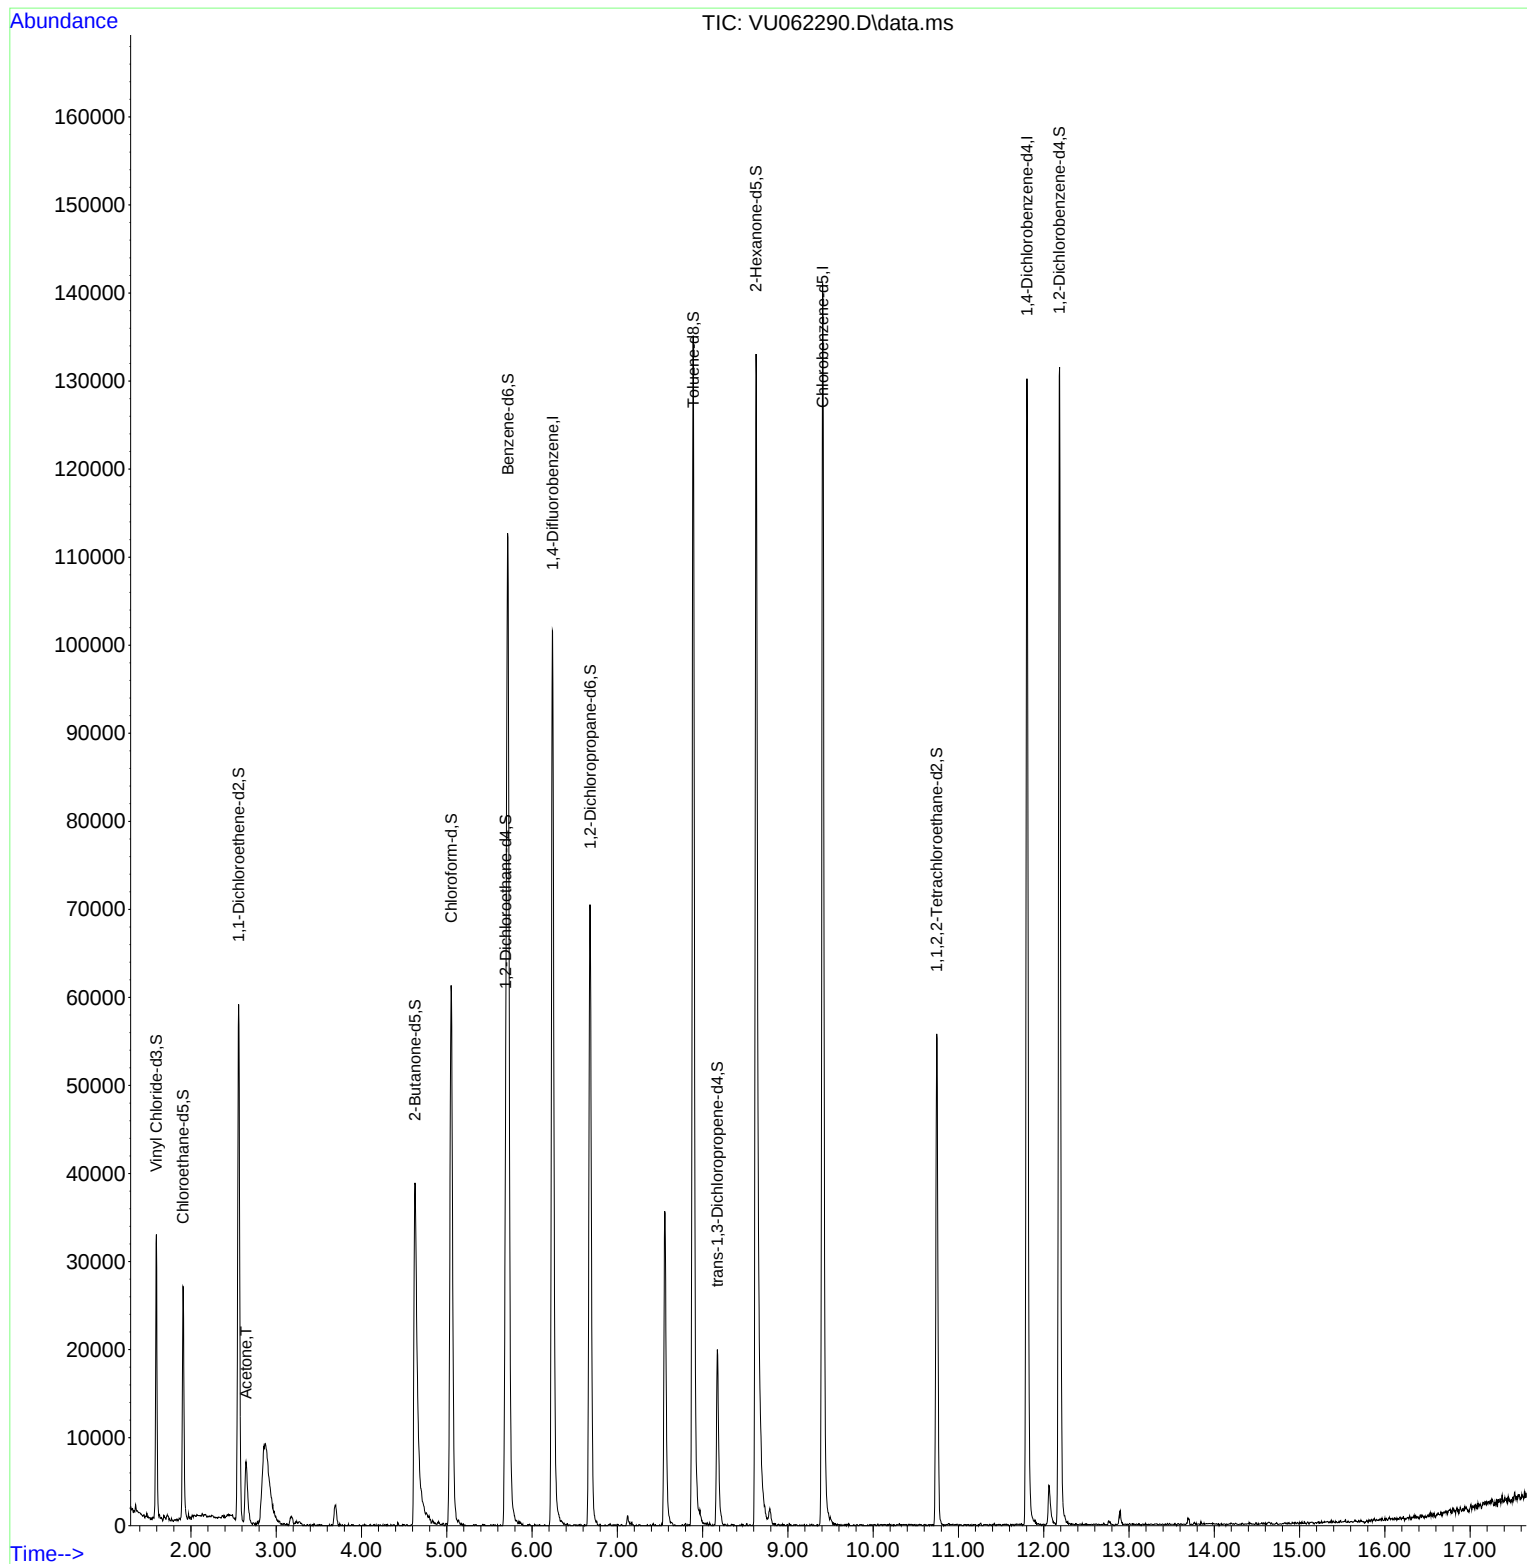

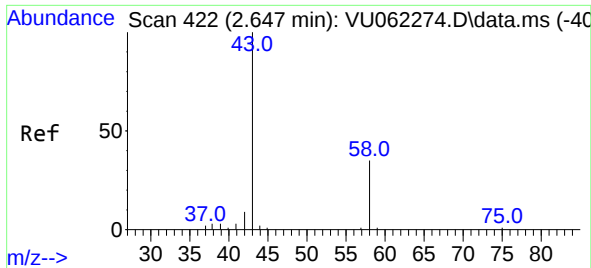

#13  
 Acetone  
 Concen: 13.339 ug/L  
 RT: 2.647 min Scan# 41  
 Delta R.T. 0.000 min  
 Lab File: VU062290.D  
 Acq: 12 Dec 2024 16:06

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 F7J56

Tgt Ion: 43 Resp: 10323  
 Ion Ratio Lower Upper  
 43 100  
 58 33.7 0.0 64.0

