


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121224\
Data File : VU062273.D
Acq On : 12 Dec 2024 08:07
Operator : MD/SY
Sample : BFB045
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB045

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Dec 13 00:13:55 2024

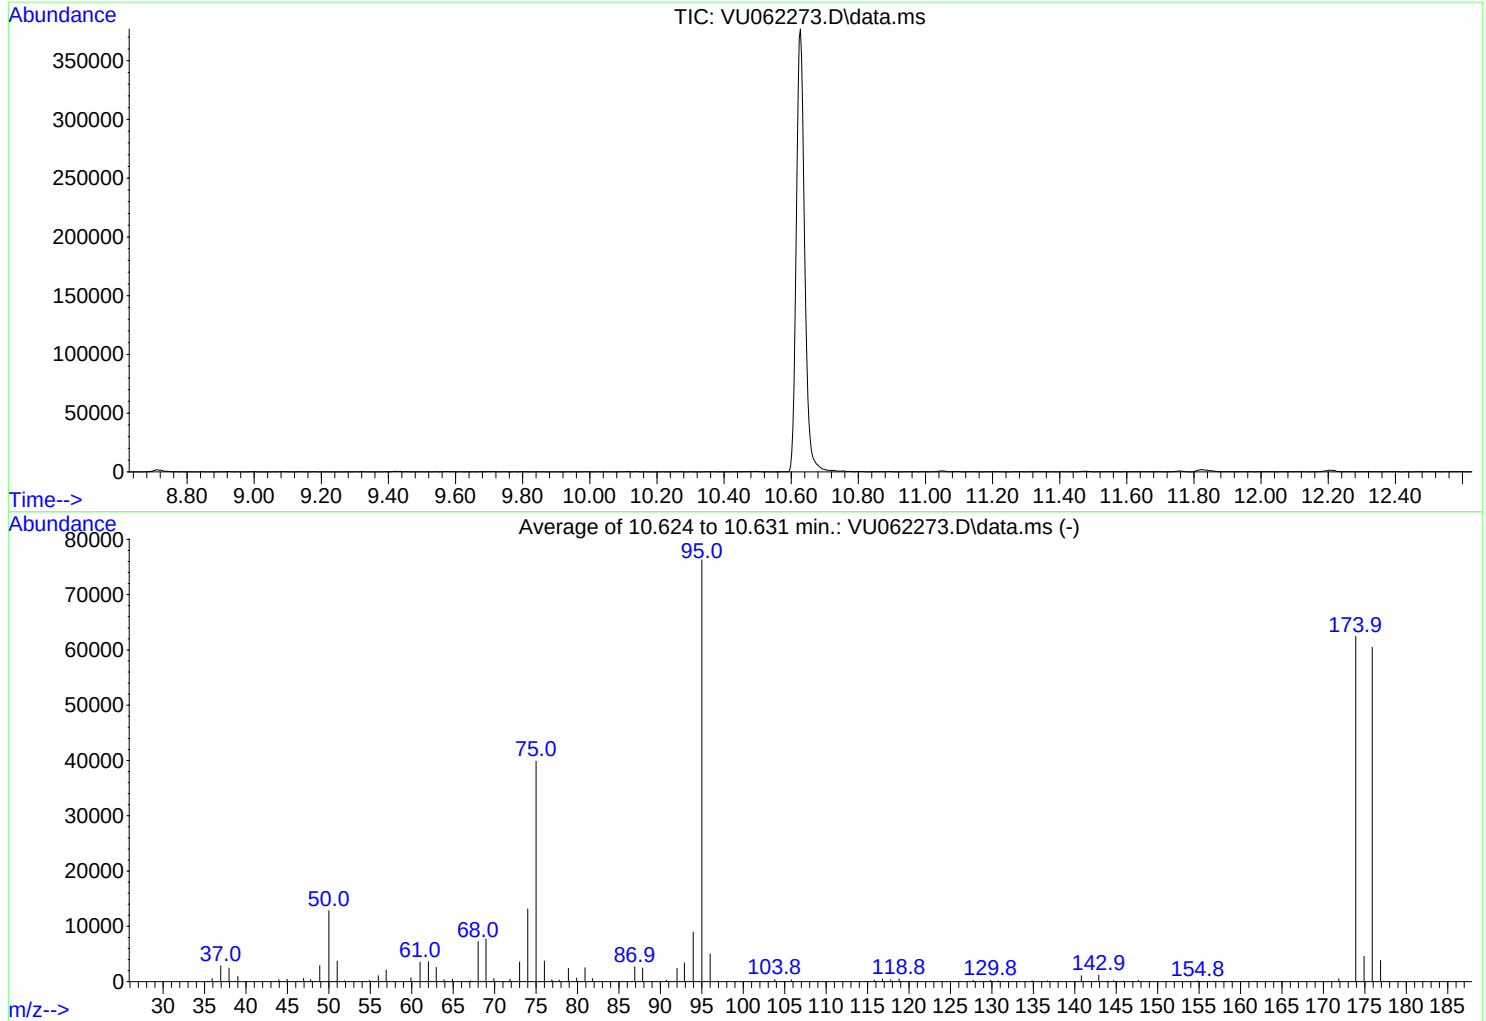

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	12844	PASS
75	95	30	80	52.3	39880	PASS
95	95	100	100	100.0	76291	PASS
96	95	5	9	6.6	4999	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	81.8	62416	PASS
175	174	5	9	7.3	4575	PASS
176	174	95	101	96.9	60485	PASS
177	176	5	9	6.3	3813	PASS

m/z	Abundance
43.90	109.0

Instrument :
MSVOA_U
ClientSampleId :
BFB045

m/z	Abundance
35.90	529.0
36.90	2895.0
37.90	2578.0
39.00	946.0
44.00	437.0
44.90	450.0
47.00	576.0
47.80	355.0
48.90	3134.0
50.00	13192.0
51.00	3864.0
51.90	125.0
54.90	217.0
56.00	1016.0
56.90	2166.0
59.90	785.0
61.00	3603.0
62.00	3695.0
63.00	2734.0
63.90	361.0
64.90	473.0
67.10	303.0
68.00	7279.0
69.00	7786.0
69.90	600.0
71.80	491.0
73.00	3498.0
74.00	13537.0
75.00	40640.0
76.00	4000.0
76.90	382.0
77.80	250.0
78.90	2499.0
79.90	714.0
80.90	2535.0
81.80	582.0
86.90	2844.0
87.90	2488.0
90.80	271.0
92.00	2381.0
92.90	3552.0
94.00	9145.0
95.00	77192.0
96.00	5213.0
97.00	132.0
103.80	463.0
104.70	127.0
105.80	354.0
115.80	277.0
116.80	545.0
117.80	301.0
118.80	548.0
127.80	227.0
128.90	115.0
129.80	239.0
130.70	162.0
134.80	193.0
136.70	165.0
140.80	1009.0
142.90	1123.0
143.80	100.0
144.70	230.0
145.90	107.0
147.70	202.0
154.80	156.0
156.80	128.0
158.90	118.0
160.90	116.0
171.80	529.0
173.90	61984.0
174.90	4460.0
175.90	59256.0
176.90	3652.0

Instrument :
MSVOA_U
ClientSampleId :
BFB045

m/z	Abundance
35.90	570.0
37.00	2928.0
38.00	2523.0
39.00	954.0
44.00	471.0
44.90	478.0
47.00	585.0
47.80	367.0
48.90	2956.0
50.00	13213.0
51.00	3856.0
51.90	142.0
54.90	234.0
56.00	1142.0
56.90	2197.0
57.80	101.0
59.90	729.0
61.00	3615.0
62.00	3749.0
63.00	2615.0
63.90	361.0
64.90	480.0
67.10	254.0
68.00	7501.0
68.90	7995.0
69.90	568.0
71.80	447.0
73.00	3696.0
74.00	13398.0
75.00	40800.0
76.00	3836.0
76.90	356.0
77.80	317.0
78.90	2507.0
79.90	700.0
80.90	2586.0
81.80	579.0
86.90	2713.0
87.80	2497.0
90.80	281.0
92.00	2498.0
92.90	3479.0
94.00	9183.0
95.00	78400.0
96.00	5087.0
96.90	115.0
103.80	413.0
105.80	331.0
114.60	100.0
115.80	287.0
116.80	507.0
117.80	340.0
118.80	502.0
127.70	259.0
128.90	117.0
129.80	249.0
130.80	185.0
134.80	179.0
136.70	162.0
139.90	105.0
140.80	1078.0
142.90	1215.0
143.90	130.0
144.70	270.0
145.90	143.0
147.70	237.0
154.80	165.0
156.80	103.0
158.90	126.0
171.80	538.0
173.90	64056.0
174.90	4713.0
175.90	62368.0
176.90	3908.0
177.90	104.0

Instrument :
MSVOA_U
ClientSampleId :
BFB045

m/z	Abundance
35.90	537.0
37.00	2758.0
38.00	2308.0
39.00	942.0
44.00	461.0
45.00	446.0
46.90	586.0
47.80	375.0
48.90	2593.0
50.00	12127.0
51.00	3474.0
51.90	142.0
54.90	225.0
55.90	1095.0
56.90	1973.0
59.90	608.0
61.00	3361.0
62.00	3424.0
62.90	2385.0
63.90	309.0
64.90	435.0
66.80	204.0
68.00	7038.0
69.00	7384.0
69.90	509.0
71.90	404.0
73.00	3512.0
74.00	12470.0
75.00	38200.0
76.00	3394.0
76.90	319.0
77.80	317.0
78.90	2246.0
79.90	622.0
80.90	2437.0
81.80	509.0
86.90	2510.0
87.80	2398.0
90.70	246.0
92.00	2367.0
92.90	3186.0
93.90	8570.0
95.00	73280.0
96.00	4698.0
96.90	100.0
103.80	356.0
105.80	277.0
115.80	291.0
116.80	462.0
117.80	369.0
118.80	504.0
127.70	272.0
129.90	297.0
130.70	188.0
134.90	170.0
136.70	128.0
140.80	1095.0
141.80	111.0
142.90	1190.0
144.00	103.0
144.70	230.0
145.90	127.0
147.70	240.0
154.90	157.0
171.90	523.0
173.90	61208.0
174.90	4552.0
175.90	59832.0
176.90	3879.0

Instrument :
MSVOA_U
ClientSampleId :
BFB045