

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121324\
 Data File : VU062300.D
 Acq On : 13 Dec 2024 10:06
 Operator : MD/SY
 Sample : P5253-13
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7J56

Quant Time: Dec 14 03:46:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 14 03:45:56 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	113631	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	108001	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	49296	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	24169	3.153	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	63.000%
7) Chloroethane-d5	1.911	69	20483	3.757	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	75.200%
11) 1,1-Dichloroethene-d2	2.563	65	11486	3.150	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.000%
20) 2-Butanone-d5	4.631	46	66394	45.200	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.400%
24) Chloroform-d	5.052	84	62949	3.795	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	75.800%
26) 1,2-Dichloroethane-d4	5.695	65	33661	4.127	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.600%
32) Benzene-d6	5.718	84	111362	3.580	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	71.600%
36) 1,2-Dichloropropane-d6	6.682	67	33505	3.765	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	75.200%
41) Toluene-d8	7.891	98	98340	3.347	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	67.000%#
43) trans-1,3-Dichloroprop...	8.174	79	14318	3.655	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.000%
46) 2-Hexanone-d5	8.627	63	47558	40.239	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.480%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	27952	4.036	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	80.800%
66) 1,2-Dichlorobenzene-d4	12.184	152	38236	4.209	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	84.200%
Target Compounds						Qvalue
13) Acetone	2.653	43	13889	13.887	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121324\
Data File : VU062300.D
Acq On : 13 Dec 2024 10:06
Operator : MD/SY
Sample : P5253-13
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7J56

Quant Time: Dec 14 03:46:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Dec 14 03:45:56 2024
Response via : Initial Calibration

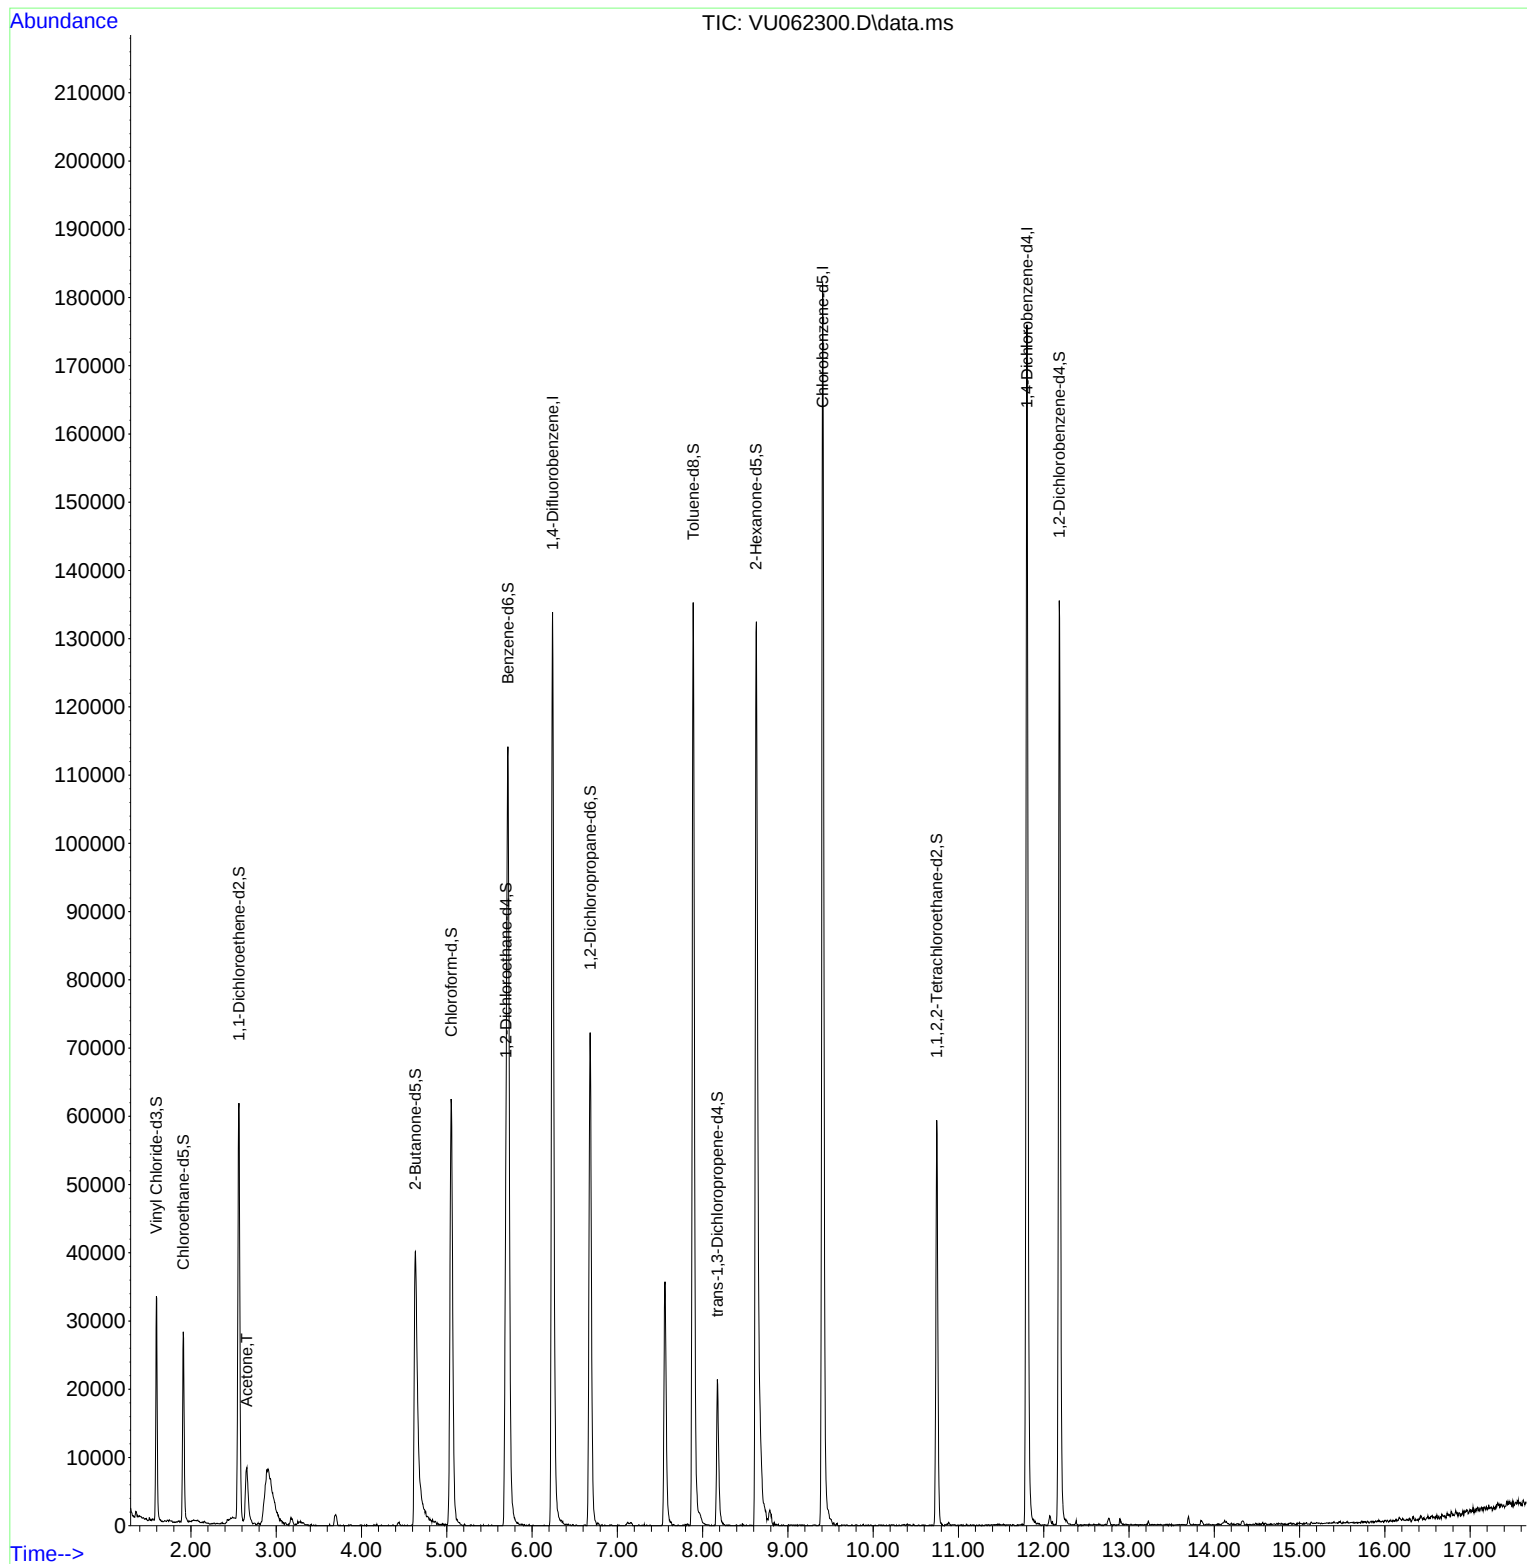

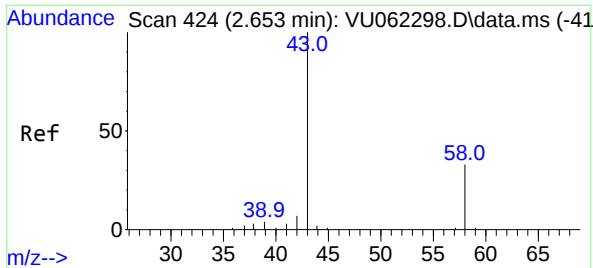

Acetone
 Concen: 13.887 ug/L
 RT: 2.653 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: VU062300.D
 Acq: 13 Dec 2024 10:06

Instrument :
 MSVOA_U
 ClientSampleId :
 F7J56

Tgt Ion:	43	Resp:	13889
Ion	Ratio	Lower	Upper
43	100		
58	31.2	0.0	64.0

