

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121324\
 Data File : VU062308.D
 Acq On : 13 Dec 2024 13:20
 Operator : MD/SY
 Sample : P5262-01
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E2AS8

Quant Time: Dec 14 03:48:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 14 03:45:56 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	85948	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	80318	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	37830	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	18976	3.273	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	65.400%
7) Chloroethane-d5	1.911	69	16801	4.074	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.400%
11) 1,1-Dichloroethene-d2	2.563	65	9614	3.486	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.800%
20) 2-Butanone-d5	4.631	46	51386	46.250	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.500%
24) Chloroform-d	5.052	84	50803	4.049	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.000%
26) 1,2-Dichloroethane-d4	5.692	65	27908	4.523	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.400%
32) Benzene-d6	5.717	84	89897	3.886	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	77.800%
36) 1,2-Dichloropropane-d6	6.679	67	28006	4.231	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.600%
41) Toluene-d8	7.891	98	78096	3.574	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.400%
43) trans-1,3-Dichloroprop...	8.174	79	11097	3.809	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.200%
46) 2-Hexanone-d5	8.627	63	39302	44.715	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.440%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	22956	4.457	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.200%
66) 1,2-Dichlorobenzene-d4	12.183	152	31228	4.480	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.600%
Target Compounds						Qvalue
16) Methylene chloride	3.042	84	6202	1.018	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121324\
Data File : VU062308.D
Acq On : 13 Dec 2024 13:20
Operator : MD/SY
Sample : P5262-01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E2AS8


Quant Time: Dec 14 03:48:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Dec 14 03:45:56 2024
Response via : Initial Calibration

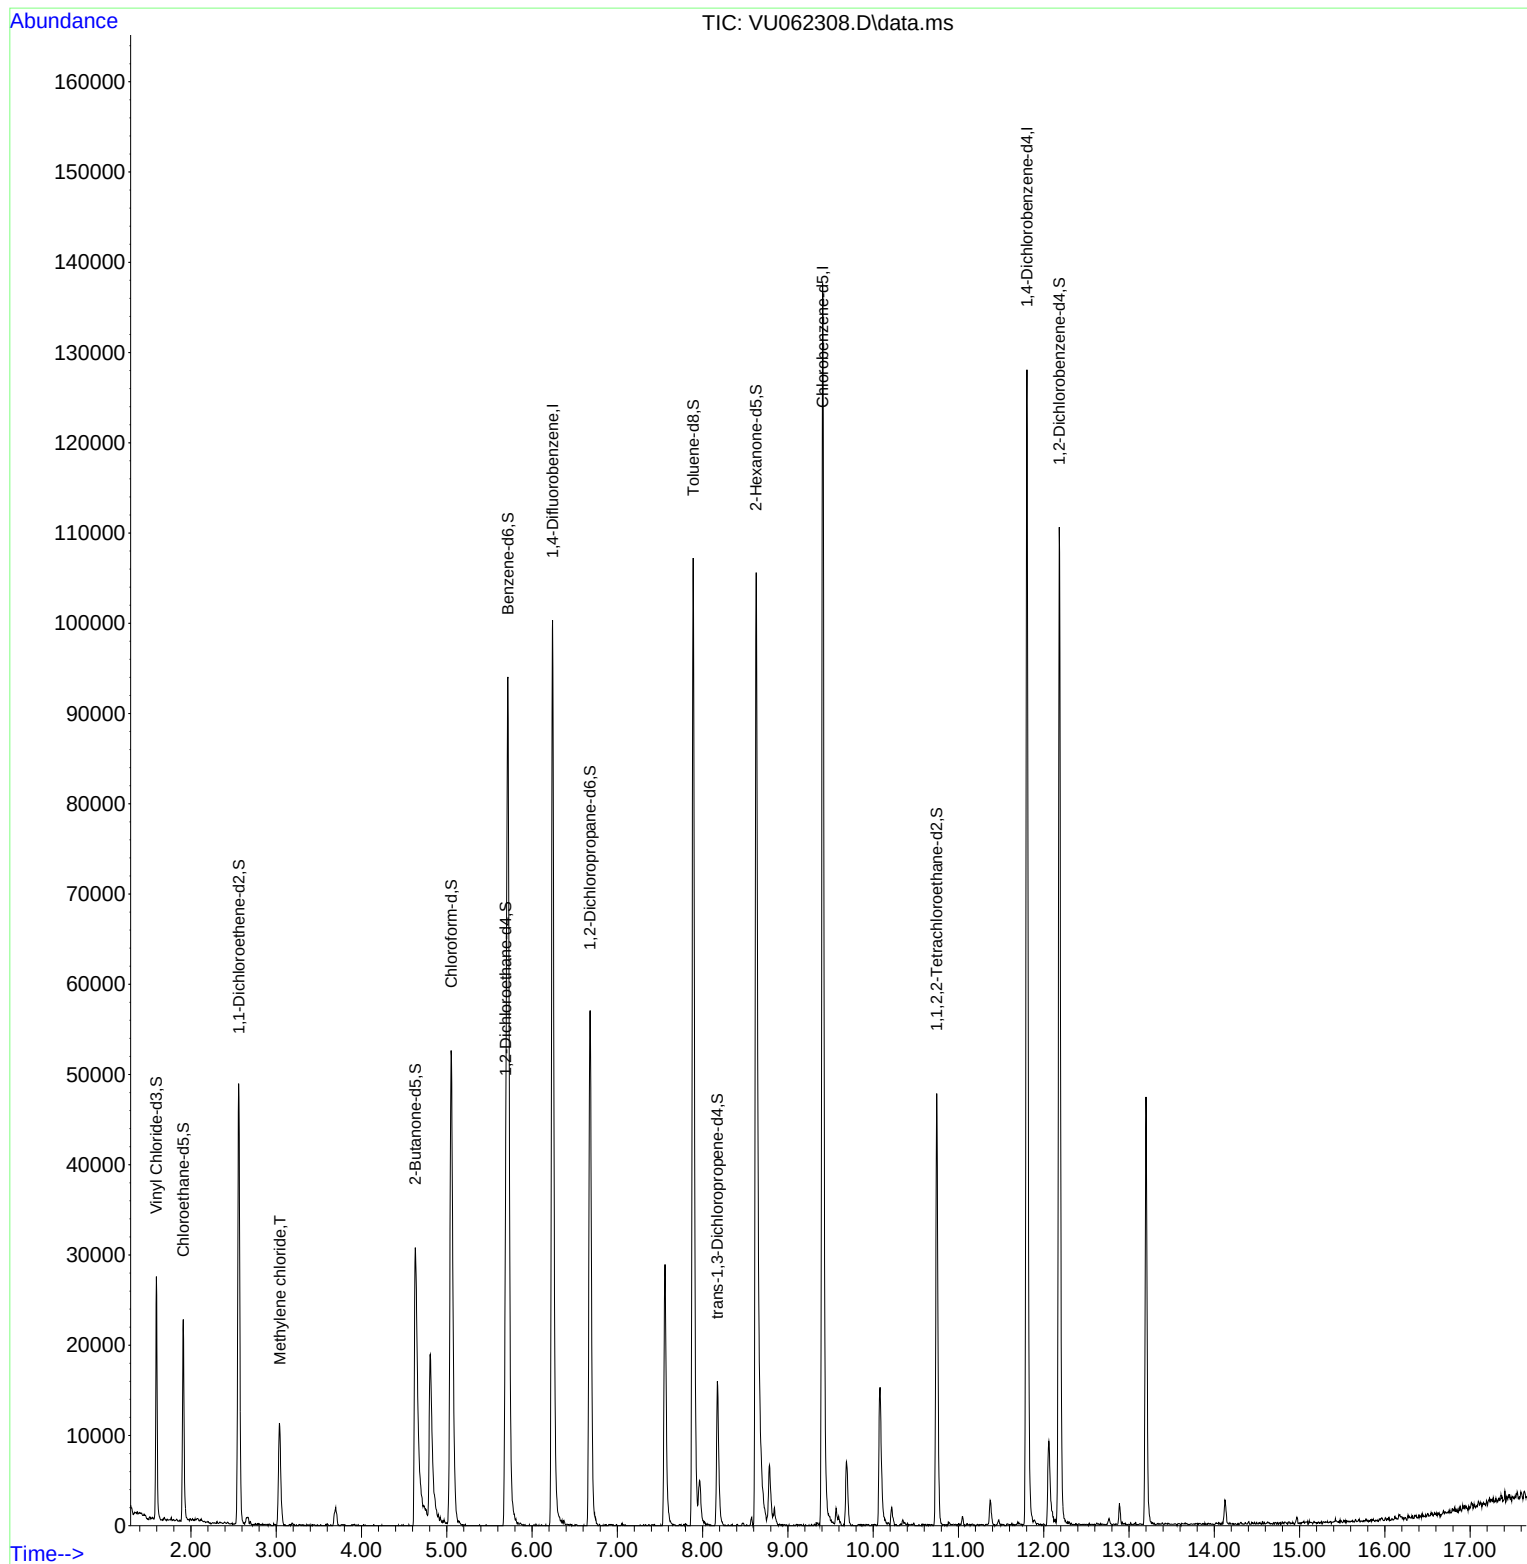

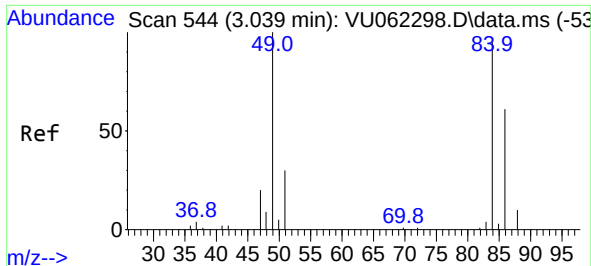

#16
Methylene chloride
Concen: 1.018 ug/L
RT: 3.042 min Scan# 54
Delta R.T. 0.003 min
Lab File: VU062308.D
Acq: 13 Dec 2024 13:20

Instrument :
MSVOA_U
ClientSampleId :
E2AS8

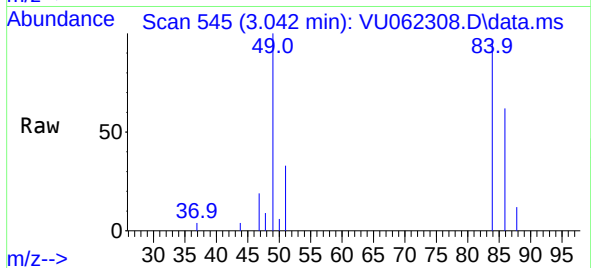

Tgt Ion: 84 Resp: 6202

Ion	Ratio	Lower	Upper
84	100		
86	65.1	43.5	80.7
49	105.1	81.9	152.1

