

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121324\
 Data File : VU062314.D
 Acq On : 13 Dec 2024 15:47
 Operator : MD/SY
 Sample : P5269-02
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7J37

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU062314.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	113	rVB	28652	32673	11.75%	1.413%
2	1.911	185	193	205	rBV	24124	32101	11.55%	1.388%
3	2.560	384	395	415	rVV	52927	86433	31.10%	3.738%
4	2.653	415	424	437	rVB2	1441	3438	1.24%	0.149%
5	3.695	739	748	756	rBV5	1919	3999	1.44%	0.173%
6	4.631	1028	1039	1069	rBV	37035	103511	37.24%	4.477%
7	5.055	1151	1171	1195	rBV	55329	125735	45.23%	5.438%
8	5.714	1358	1376	1403	rBV3	102398	271626	97.72%	11.747%
9	6.242	1528	1540	1561	rBV	95892	189727	68.26%	8.205%
10	6.544	1624	1634	1644	rBB5	3281	6281	2.26%	0.272%
11	6.679	1665	1676	1697	rBV	63904	127366	45.82%	5.508%
12	7.560	1940	1950	1972	rBV2	31790	59901	21.55%	2.591%
13	7.891	2042	2053	2078	rBV	121259	214769	77.27%	9.288%
14	8.174	2132	2141	2161	rBV2	18503	33192	11.94%	1.435%
15	8.547	2249	2257	2269	rBB5	6622	10952	3.94%	0.474%
16	8.627	2272	2282	2322	rBV2	128521	277960	100.00%	12.021%
17	9.409	2514	2525	2548	rBV	135769	236187	84.97%	10.215%
18	10.746	2930	2941	2959	rBV	53537	87528	31.49%	3.785%
19	11.804	3259	3270	3289	rBV	122406	207179	74.54%	8.960%
20	12.184	3377	3388	3414	rBV	117932	201675	72.56%	8.722%




Sum of corrected areas: 2312233

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121324\
Data File : VU062314.D
Acq On : 13 Dec 2024 15:47
Operator : MD/SY
Sample : P5269-02
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7J37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

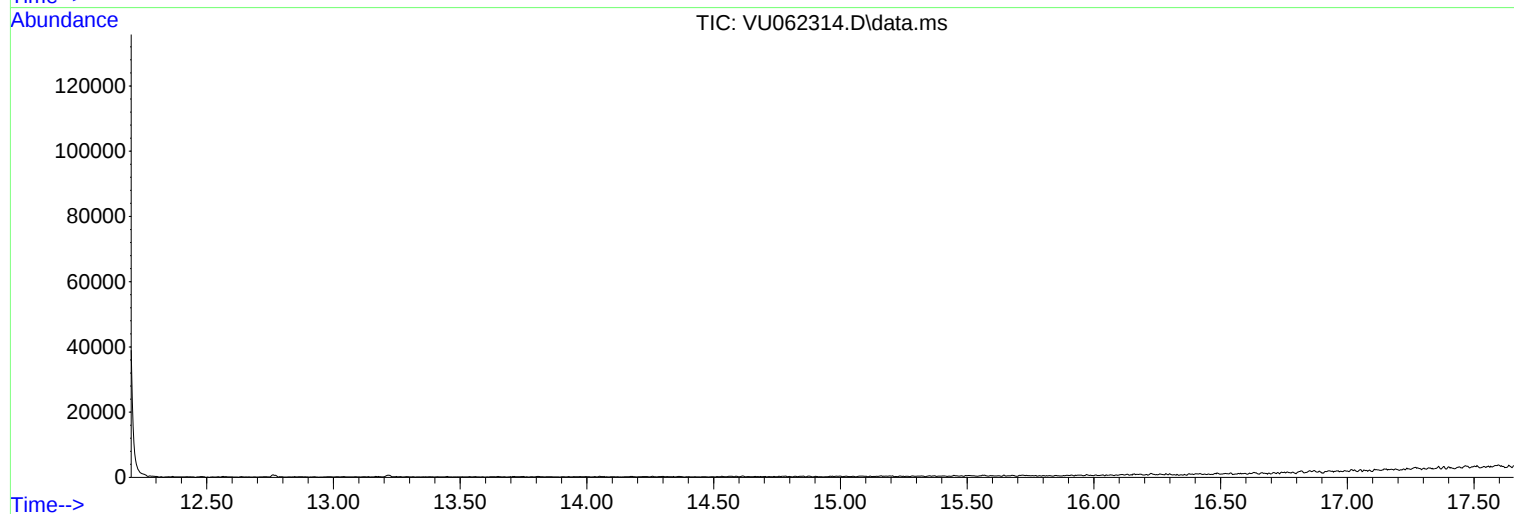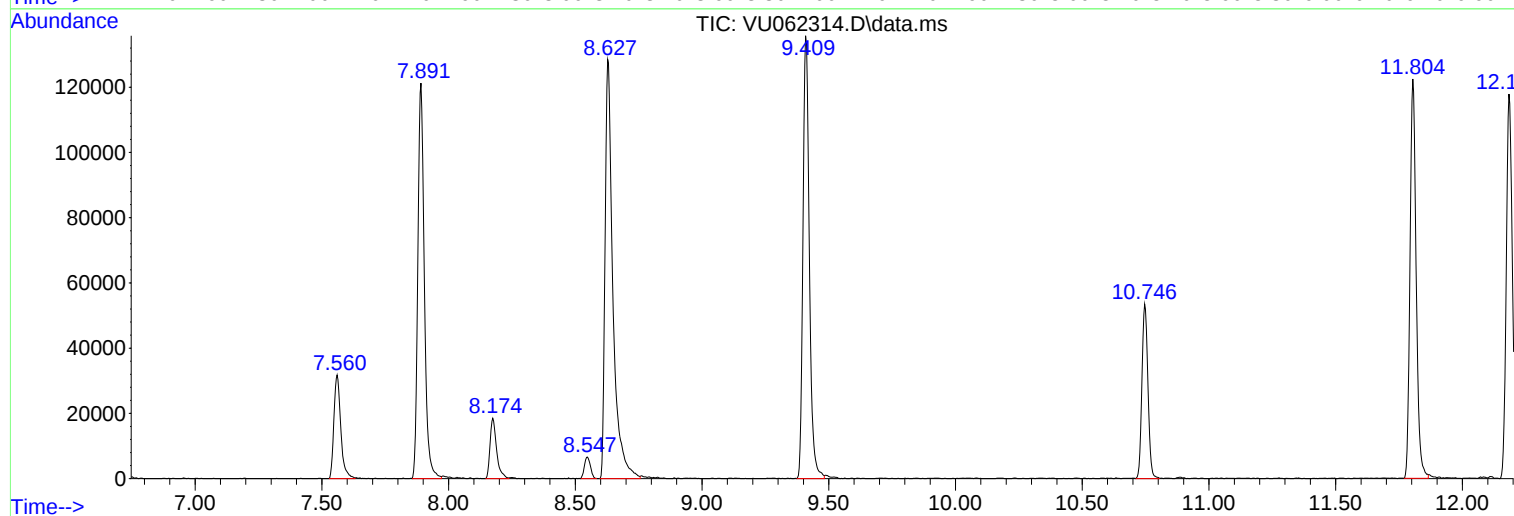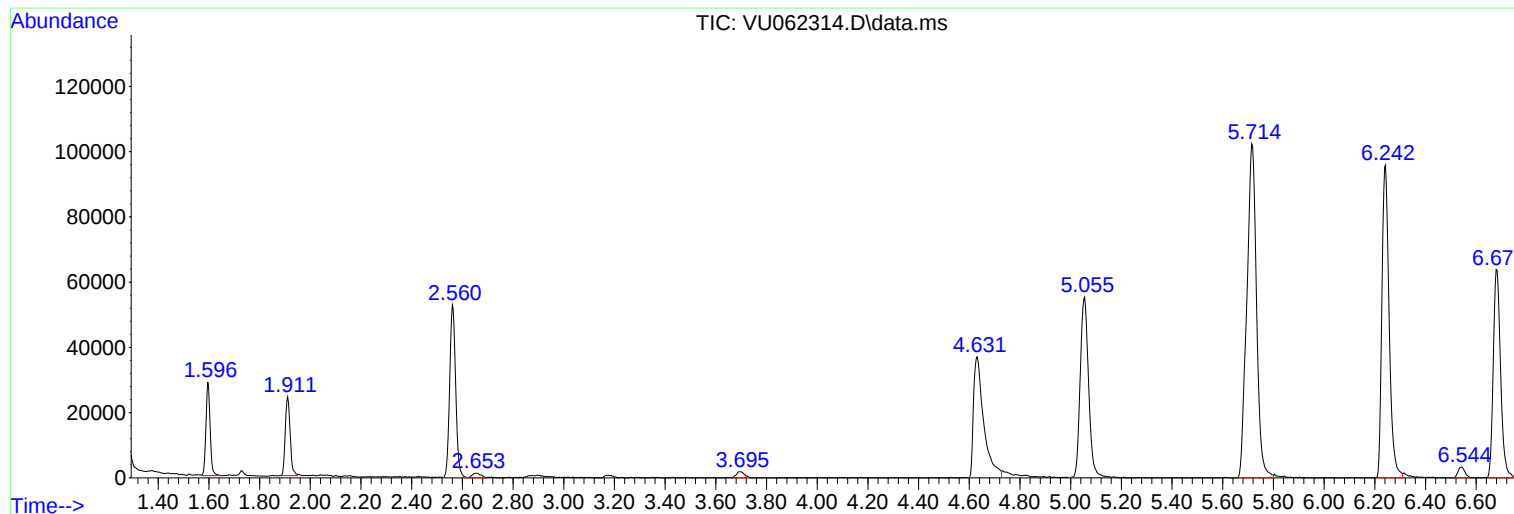

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121324\
Data File : VU062314.D
Acq On : 13 Dec 2024 15:47
Operator : MD/SY
Sample : P5269-02
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7J37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121324\
Data File : VU062314.D
Acq On : 13 Dec 2024 15:47
Operator : MD/SY
Sample : P5269-02
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7J37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc