


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121324\
Data File : VU062297.D
Acq On : 13 Dec 2024 08:09
Operator : MD/SY
Sample : BFB046
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB046

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Dec 17 01:28:58 2024

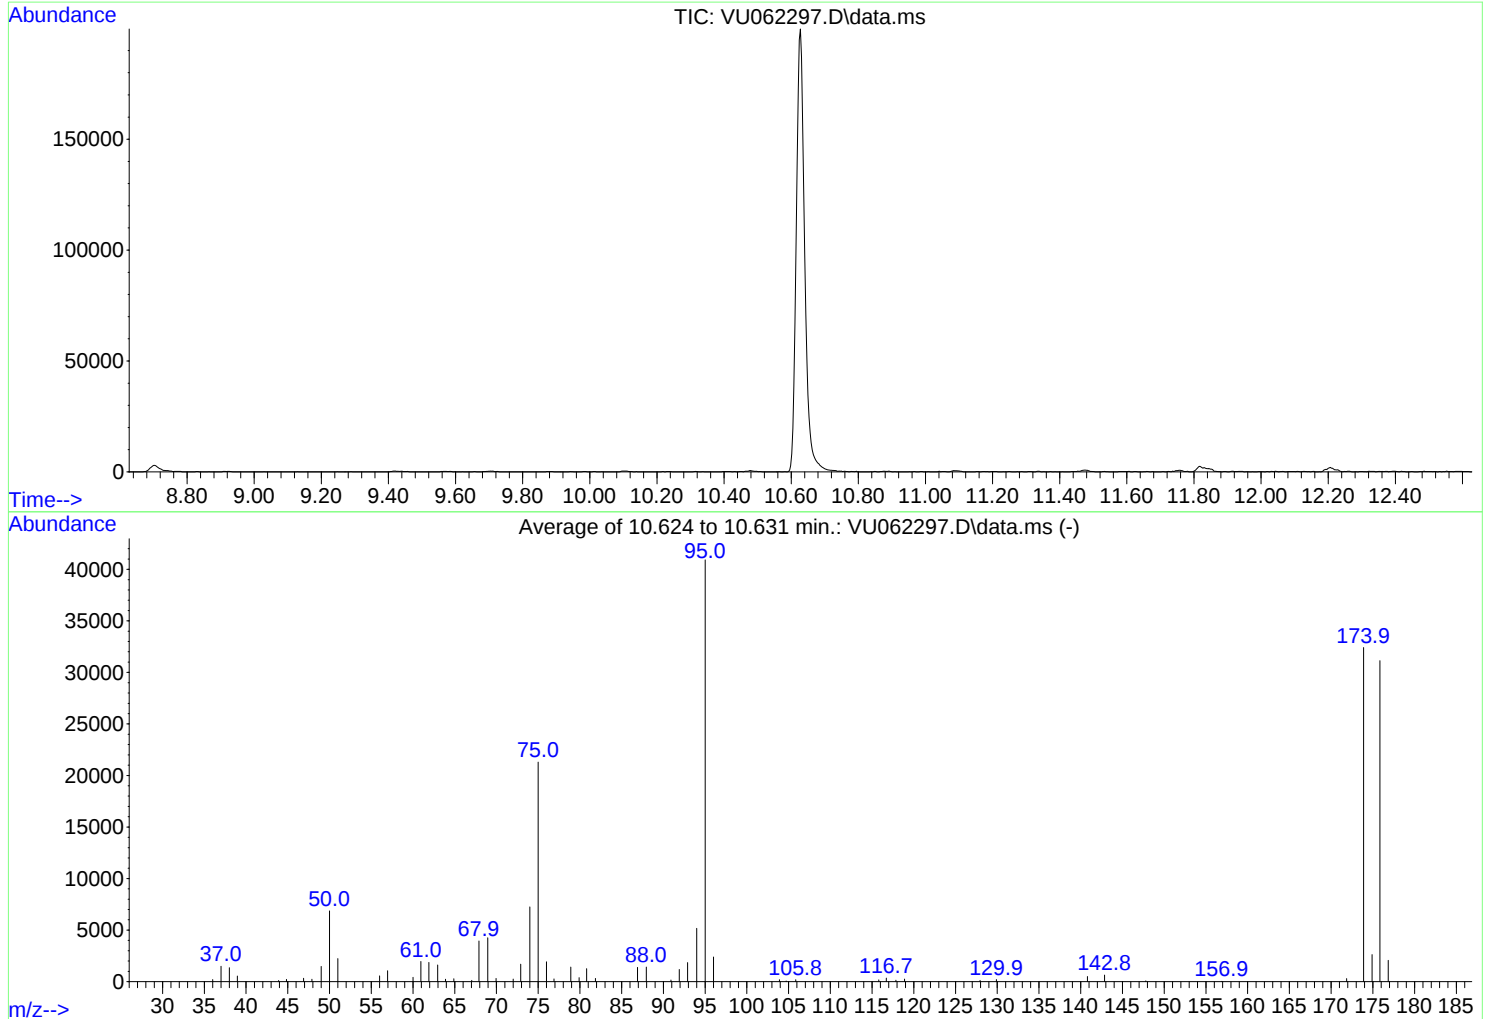

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	6858	PASS
75	95	30	80	52.0	21291	PASS
95	95	100	100	100.0	40920	PASS
96	95	5	9	5.9	2399	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.2	32419	PASS
175	174	5	9	8.1	2629	PASS
176	174	95	101	96.0	31136	PASS
177	176	5	9	6.6	2067	PASS

m/z	Abundance
43.80	110.0

Instrument :
MSVOA_U
ClientSampleId :
BFB046

m/z	Abundance
36.00	227.0
37.00	1487.0
38.00	1503.0
39.00	503.0
43.90	203.0
44.90	234.0
46.90	352.0
47.90	245.0
49.00	1610.0
50.00	7308.0
51.00	2141.0
56.00	597.0
56.90	1027.0
60.00	370.0
61.00	1981.0
61.90	1821.0
63.00	1708.0
63.90	242.0
64.90	280.0
67.10	132.0
67.90	4000.0
69.00	4398.0
69.90	372.0
72.00	243.0
72.90	1741.0
74.00	7206.0
75.00	21528.0
76.00	1984.0
76.90	249.0
78.90	1487.0
79.90	349.0
80.80	1354.0
81.80	339.0
86.90	1367.0
88.00	1446.0
90.90	172.0
91.90	1167.0
92.90	1778.0
94.00	5386.0
95.00	41248.0
96.00	2417.0
103.90	178.0
104.70	110.0
105.90	200.0
115.80	148.0
116.70	321.0
117.80	126.0
118.90	265.0
128.00	120.0
129.90	173.0
140.80	529.0
142.90	598.0
171.90	288.0
173.90	32200.0
174.90	2593.0
175.90	30600.0
176.80	2118.0

Instrument :
MSVOA_U
ClientSampleId :
BFB046

m/z	Abundance
36.00	211.0
37.00	1527.0
38.00	1383.0
38.90	557.0
44.00	233.0
44.90	216.0
46.90	320.0
47.90	226.0
49.00	1522.0
50.00	7062.0
51.00	2314.0
56.00	605.0
57.00	1117.0
60.00	433.0
61.00	2025.0
61.90	1943.0
63.00	1621.0
63.90	250.0
64.90	280.0
67.00	124.0
67.90	4071.0
69.00	4407.0
70.00	326.0
72.00	252.0
72.90	1740.0
74.00	7468.0
75.00	22056.0
76.00	2023.0
76.90	284.0
78.90	1444.0
79.90	403.0
80.80	1293.0
81.80	327.0
86.90	1418.0
88.00	1467.0
90.90	162.0
91.90	1197.0
92.90	1897.0
94.00	5360.0
95.00	42184.0
96.00	2415.0
103.90	199.0
104.70	103.0
105.80	196.0
115.80	170.0
116.70	367.0
117.90	138.0
118.90	257.0
128.00	140.0
129.90	225.0
140.80	511.0
142.80	656.0
147.80	110.0
171.80	300.0
173.90	33320.0
174.90	2676.0
175.80	32000.0
176.80	2140.0

Instrument :
MSVOA_U
ClientSampleId :
BFB046

m/z	Abundance
36.00	194.0
37.00	1452.0
38.00	1174.0
38.90	563.0
44.00	244.0
44.80	215.0
46.90	287.0
47.90	214.0
49.00	1271.0
50.00	6203.0
51.00	2260.0
56.00	499.0
56.90	1041.0
60.00	466.0
60.90	1848.0
61.90	1818.0
62.90	1501.0
63.90	206.0
64.90	279.0
67.00	128.0
67.90	3762.0
68.90	3970.0
70.00	232.0
72.00	238.0
72.90	1593.0
74.00	7057.0
75.00	20288.0
76.00	1782.0
76.90	283.0
78.90	1305.0
79.90	434.0
80.80	1144.0
81.90	281.0
86.90	1350.0
87.90	1322.0
90.90	143.0
91.90	1160.0
92.90	1854.0
94.00	4779.0
95.00	39328.0
96.00	2364.0
103.90	179.0
105.80	188.0
115.80	174.0
116.70	347.0
117.90	148.0
118.90	238.0
127.80	138.0
129.90	222.0
140.80	469.0
142.80	645.0
147.80	126.0
156.90	117.0
171.80	285.0
173.90	31736.0
174.90	2619.0
175.80	30808.0
176.90	1943.0

Instrument :
MSVOA_U
ClientSampleId :
BFB046