

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121423\
 Data File : VU056863.D
 Acq On : 15 Dec 2023 02:38
 Operator : MD/SY
 Sample : 05770-12
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Dec 15 05:12:18 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Dec 15 01:53:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	230483	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	236268	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	98315	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	54897	2.779	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	55.600%
7) Chloroethane-d5	1.911	69	56127	3.796	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.000%
11) 1,1-Dichloroethene-d2	2.563	65	26586	3.145	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.000%
20) 2-Butanone-d5	4.644	46	178384	45.721	ug/L	0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.440%
24) Chloroform-d	5.055	84	151308	4.044	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.800%
26) 1,2-Dichloroethane-d4	5.698	65	75418	4.260	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.200%
32) Benzene-d6	5.721	84	264517	3.609	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	72.200%
36) 1,2-Dichloropropane-d6	6.685	67	93524	4.077	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	81.600%
41) Toluene-d8	7.894	98	212147	3.239	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	64.800%#
43) trans-1,3-Dichloroprop...	8.177	79	29293	3.293	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	65.800%
46) 2-Hexanone-d5	8.631	63	133098	39.672	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.340%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	73036	4.401	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.000%
66) 1,2-Dichlorobenzene-d4	12.187	152	82459	4.267	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	85.400%
Target Compounds						Qvalue
3) Chloromethane	1.515	50	6553	0.276	ug/L	91
5) Vinyl chloride	1.599	62	16065	0.681	ug/L #	75
14) Carbon disulfide	2.788	76	22793	0.351	ug/L	98
15) Methyl Acetate	3.078	43	8127	1.256	ug/L #	49
22) cis-1,2-Dichloroethene	4.663	96	49799	2.413	ug/L	95
33) Benzene	5.772	78	19031	0.229	ug/L	100
34) Trichloroethene	6.537	95	14446	0.634	ug/L	94
37) 1,2-Dichloropropane	6.688	63	10016	0.472	ug/L #	1
42) Toluene	7.965	91	81833	0.952	ug/L	98
48) 2-Hexanone	8.688	43	5245	0.730	ug/L #	69
53) m,p-Xylene	9.692	106	5852	0.166	ug/L	97
61) 1,2,3-Trichloropropane	11.807	75	13557	1.284	ug/L #	68
67) 1,2-Dichlorobenzene	12.209	146	5100	0.152	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121423\
Data File : VU056863.D
Acq On : 15 Dec 2023 02:38
Operator : MD/SY
Sample : 05770-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Dec 15 05:12:18 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Dec 15 01:53:53 2023
Response via : Initial Calibration

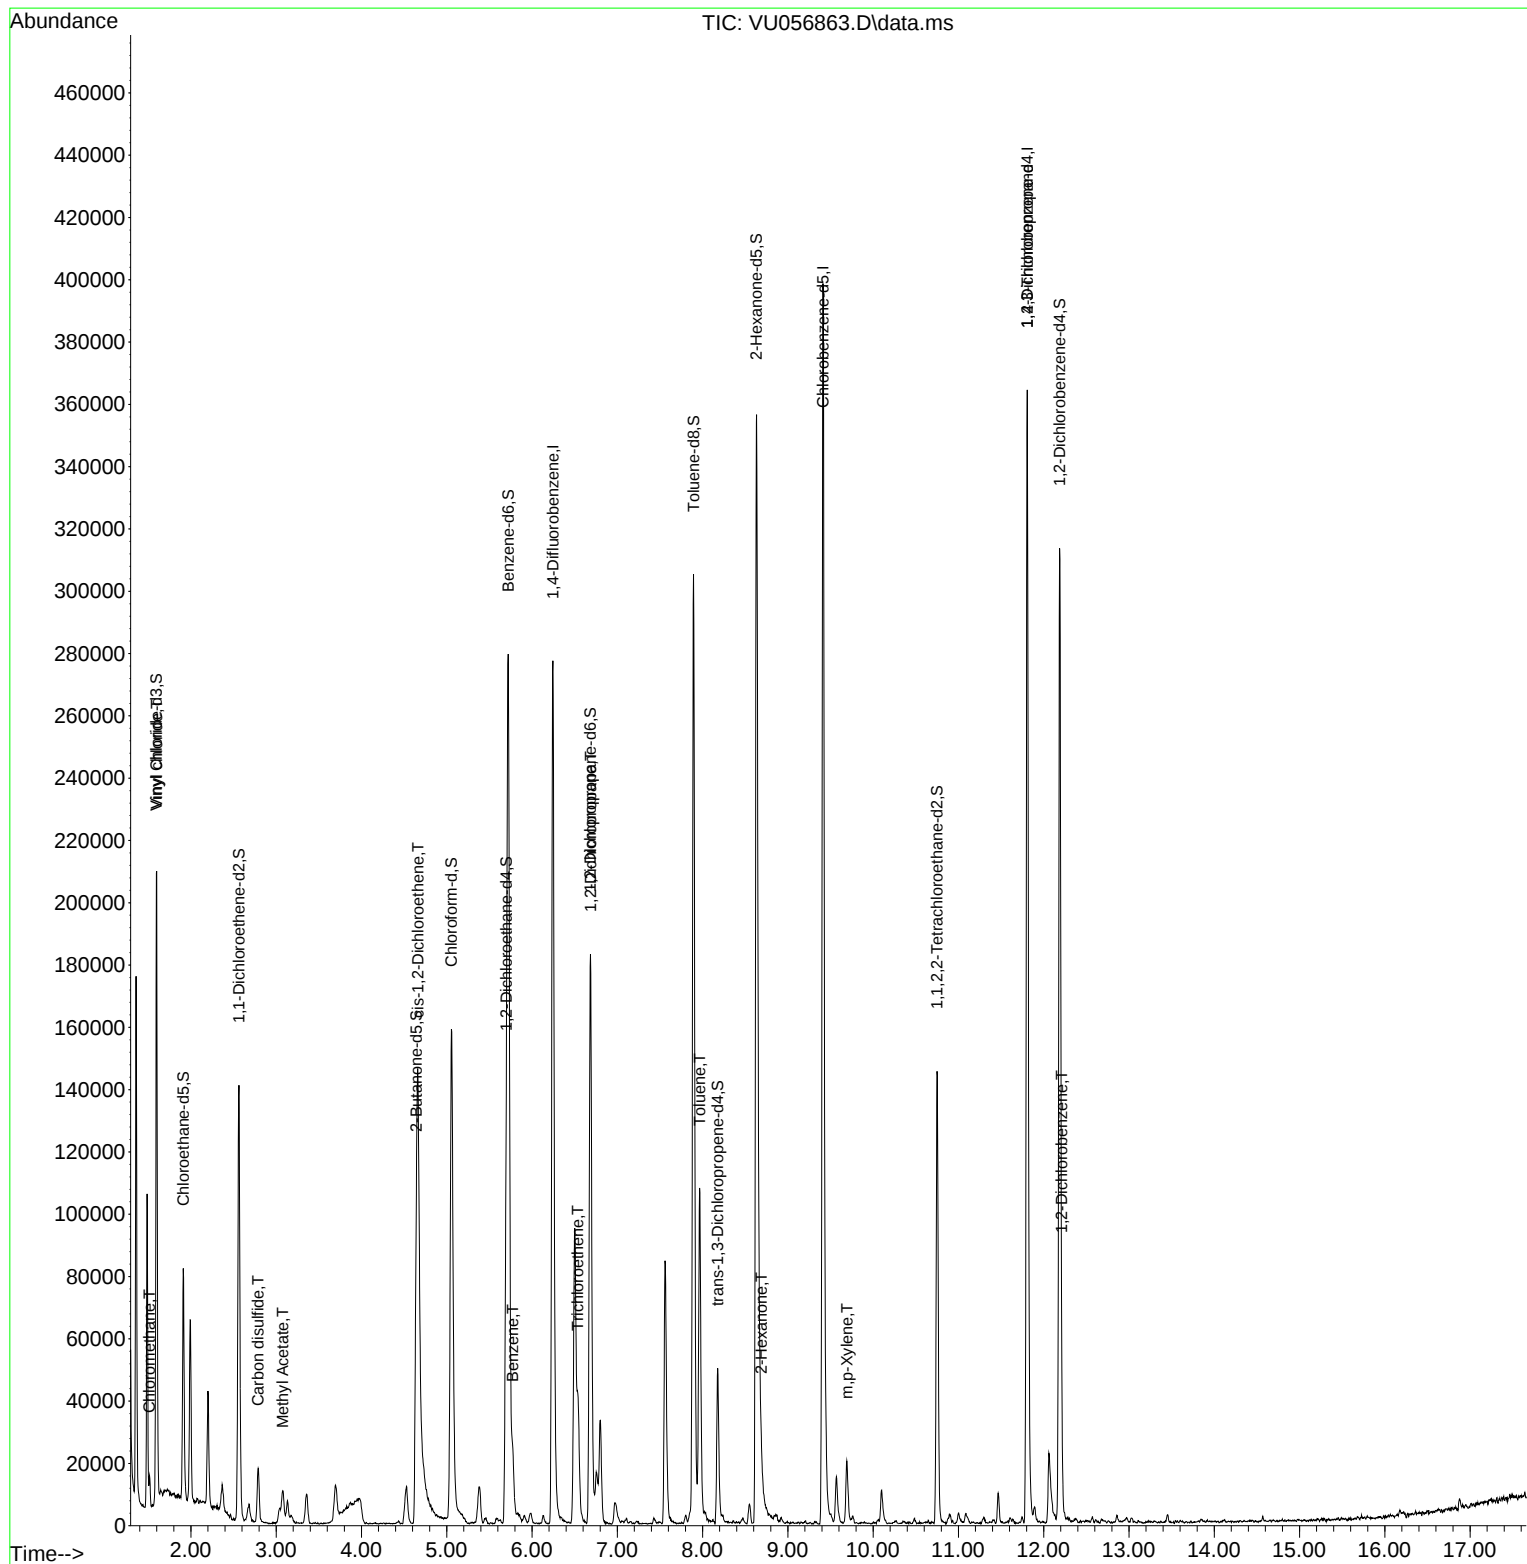

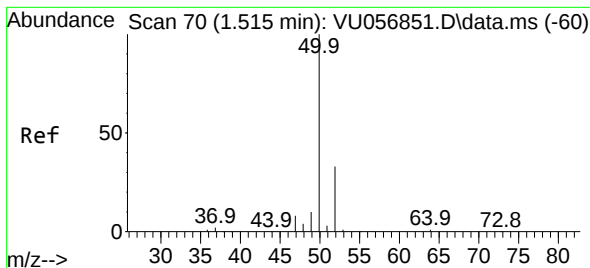

#3

Chloromethane

Concen: 0.276 ug/L

RT: 1.515 min Scan# 70

Delta R.T. -0.000 min

Lab File: VU056863.D

Acq: 15 Dec 2023 02:38

Instrument :

MSVOA_U





ClientSampleId :

Tgt Ion: 50 Resp: 6553

Ion Ratio Lower Upper

50 100

52 36.9 22.5 41.7

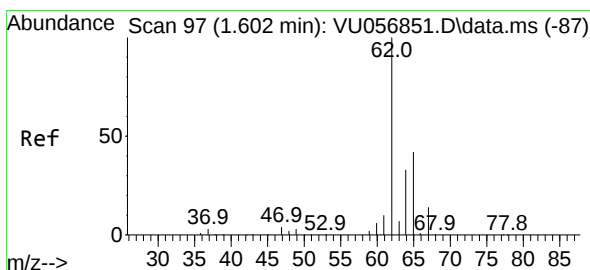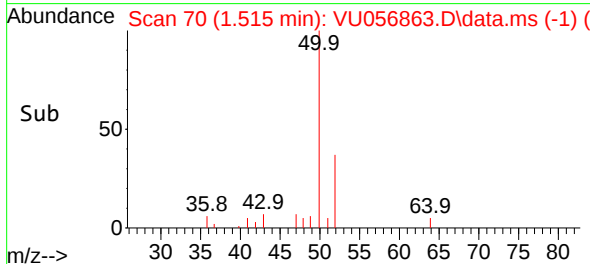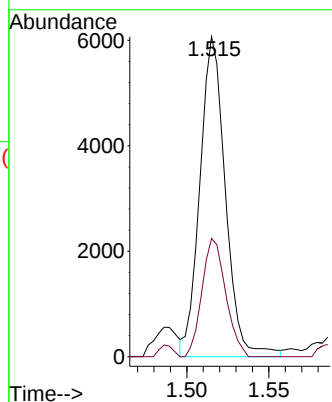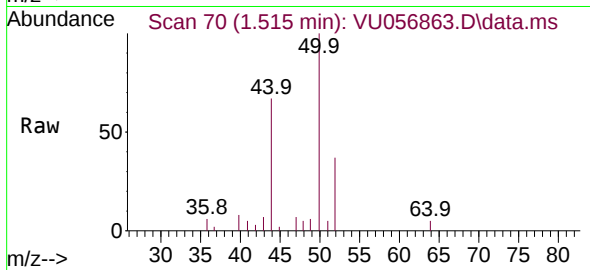

#5

Vinyl chloride

Concen: 0.681 ug/L

RT: 1.599 min Scan# 96

Delta R.T. -0.003 min

Lab File: VU056863.D




Acq: 15 Dec 2023 02:38


Tgt Ion: 62 Resp: 16065

Ion Ratio Lower Upper

62 100


64 46.9 22.8 42.4#

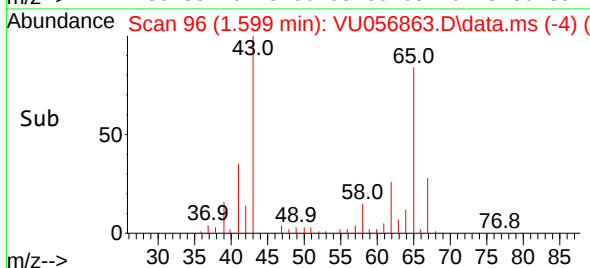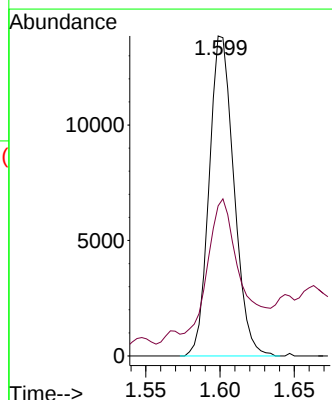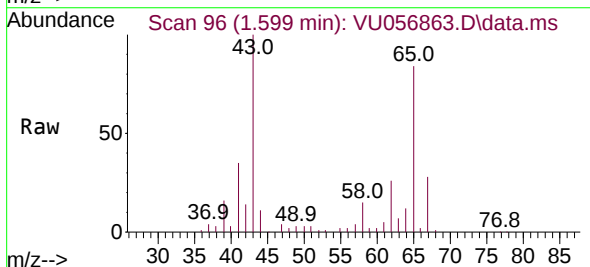



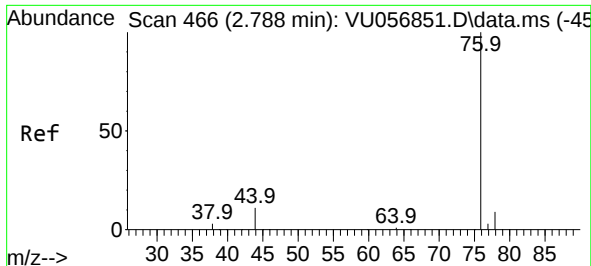


#14
Carbon disulfide
Concen: 0.351 ug/L
RT: 2.788 min Scan# 466
Delta R.T. -0.000 min
Lab File: VU056863.D
Acq: 15 Dec 2023 02:38

Instrument :
MSVOA_U
ClientSampleId :



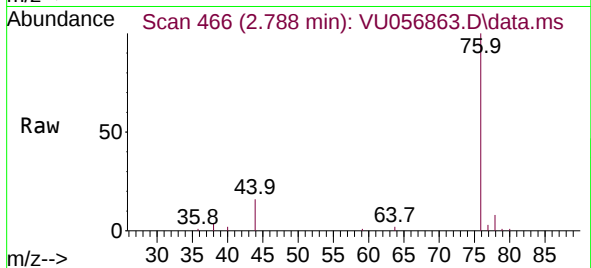



Tgt Ion: 76 Resp: 22793
Ion Ratio Lower Upper
76 100
78 8.3 7.3 10.9

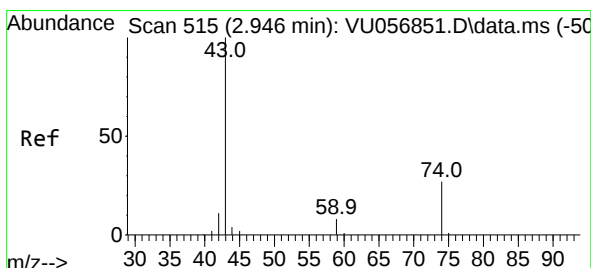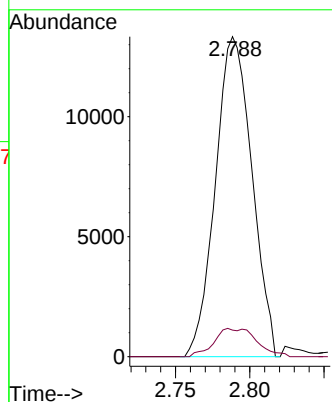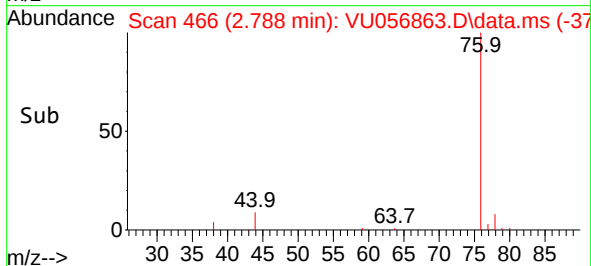

#15
Methyl Acetate
Concen: 1.256 ug/L
RT: 3.078 min Scan# 556
Delta R.T. 0.132 min
Lab File: VU056863.D
Acq: 15 Dec 2023 02:38

Tgt Ion: 43 Resp: 8127
Ion Ratio Lower Upper
43 100
74 0.0 21.0 31.6#

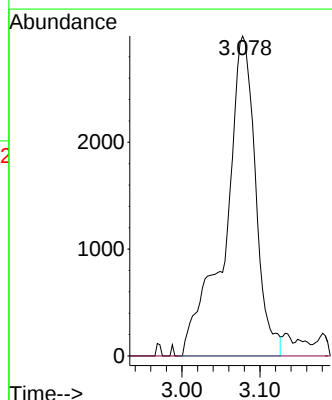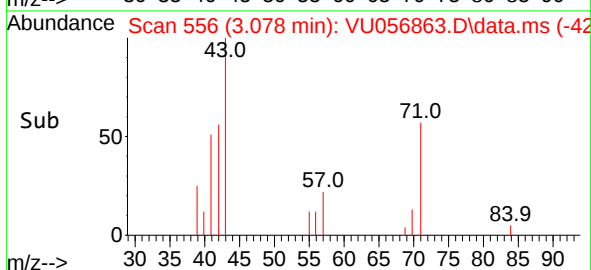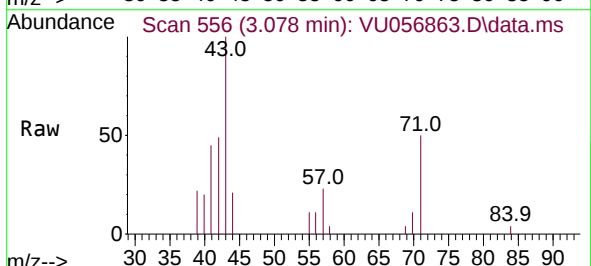

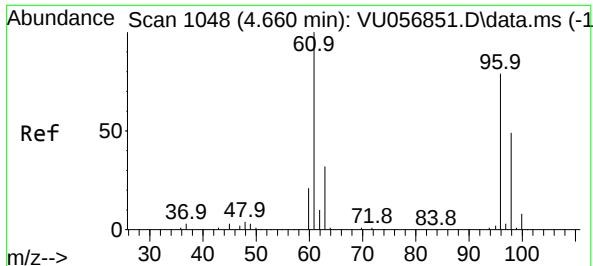

#22

cis-1,2-Dichloroethene

Concen: 2.413 ug/L

RT: 4.663 min Scan# 1049

Delta R.T. 0.003 min

Lab File: VU056863.D

Acq: 15 Dec 2023 02:38

Instrument :

MSVOA_U

ClientSampleId :





Tgt Ion: 96 Resp: 49799

Ion Ratio Lower Upper

96 100

61 123.4 91.3 169.6

98 62.0 44.2 82.0

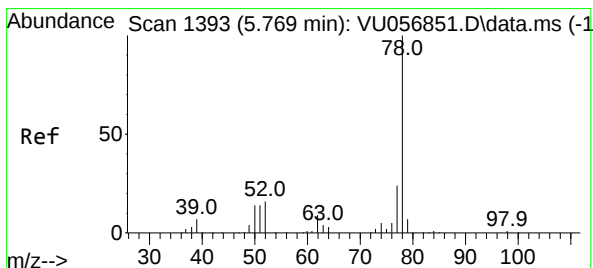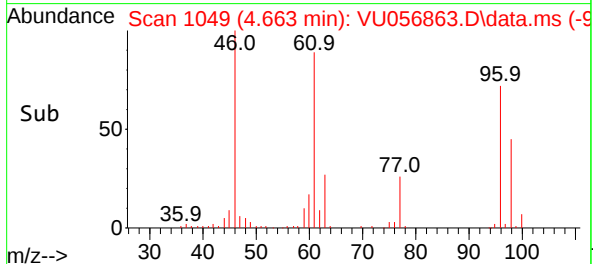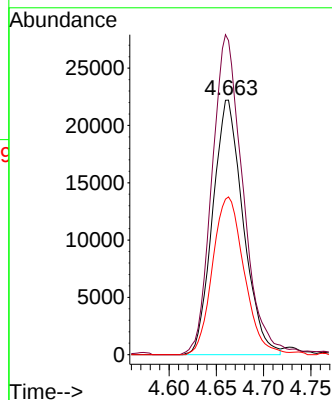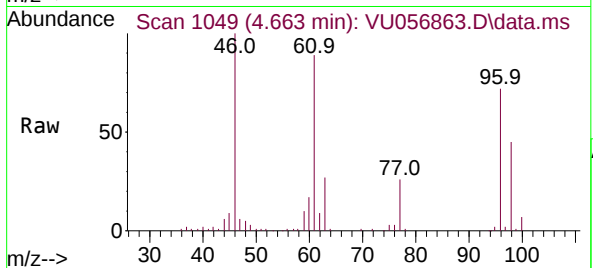

#33

Benzene

Concen: 0.229 ug/L




RT: 5.772 min Scan# 1394


Delta R.T. 0.003 min

Lab File: VU056863.D

Acq: 15 Dec 2023 02:38

Tgt Ion: 78 Resp: 19031

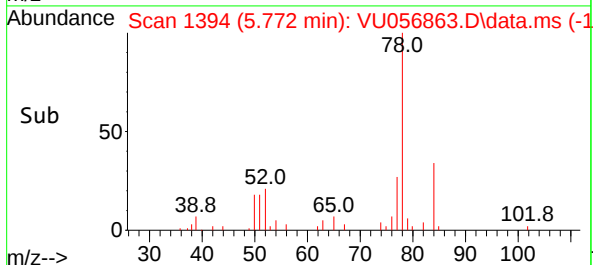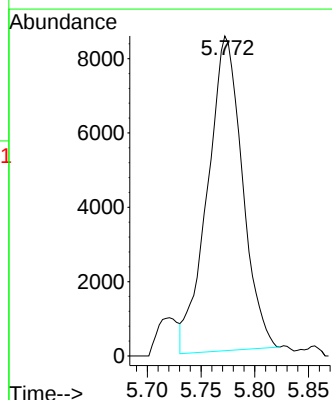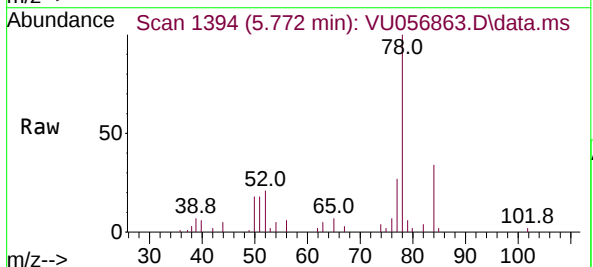




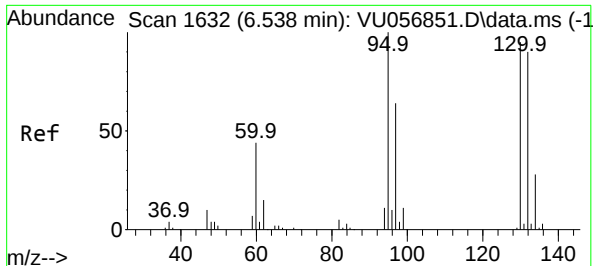


#34
 Trichloroethene
 Concen: 0.634 ug/L
 RT: 6.537 min Scan# 1632
 Delta R.T. -0.000 min
 Lab File: VU056863.D
 Acq: 15 Dec 2023 02:38

Instrument :
 MSVOA_U
 ClientSampleId :

Tgt Ion: 95 Resp: 14446




Ion	Ratio	Lower	Upper
95	100		
97	67.9	46.1	85.5
132	83.7	63.6	118.0
130	88.1	66.4	123.4

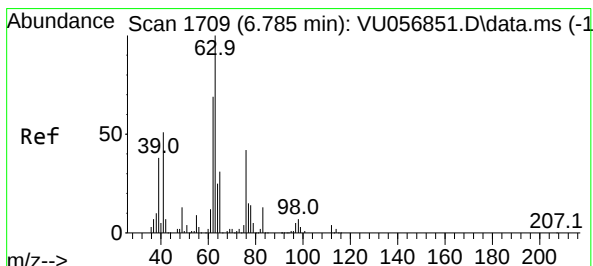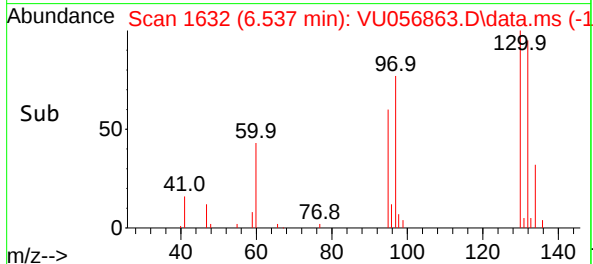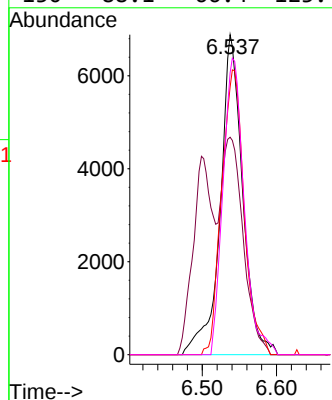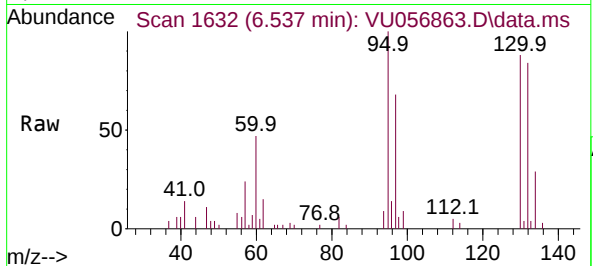


#37
 1,2-Dichloropropane
 Concen: 0.472 ug/L
 RT: 6.688 min Scan# 1679
 Delta R.T. -0.097 min
 Lab File: VU056863.D
 Acq: 15 Dec 2023 02:38

Tgt Ion: 63 Resp: 10016

Ion	Ratio	Lower	Upper
63	100		
112	41.5	3.3	4.9#

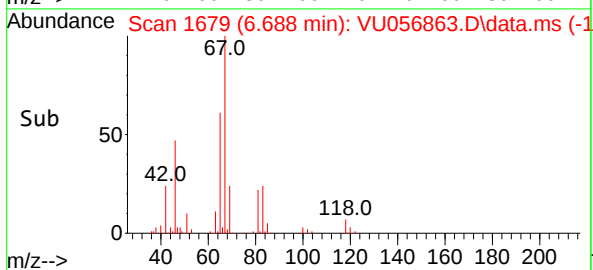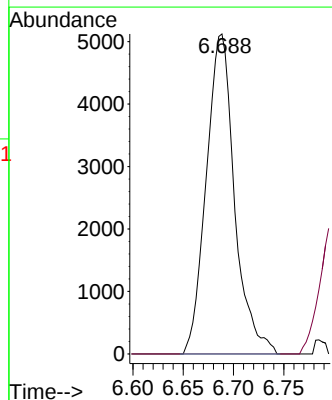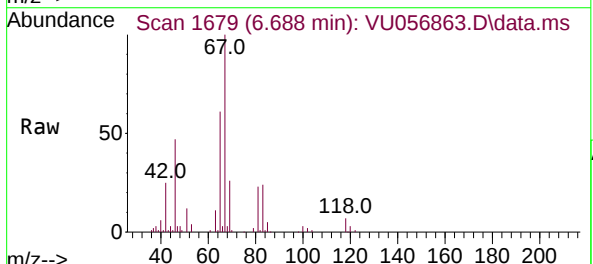

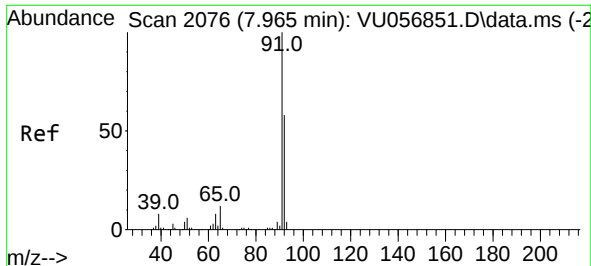

#42

Toluene

Concen: 0.952 ug/L

RT: 7.965 min Scan# 2076

Delta R.T. -0.000 min

Lab File: VU056863.D

Acq: 15 Dec 2023 02:38

Instrument :

MSVOA_U





ClientSampleId :

Tgt Ion: 91 Resp: 81833

Ion Ratio Lower Upper

91 100

92 59.0 40.4 75.0

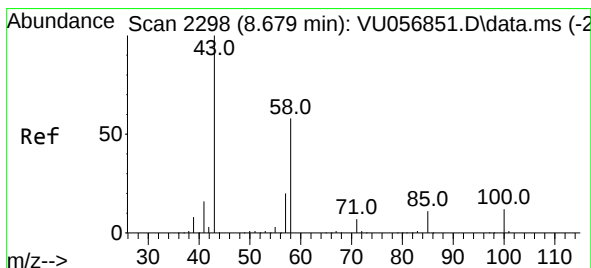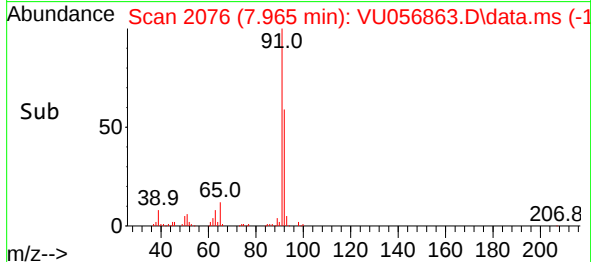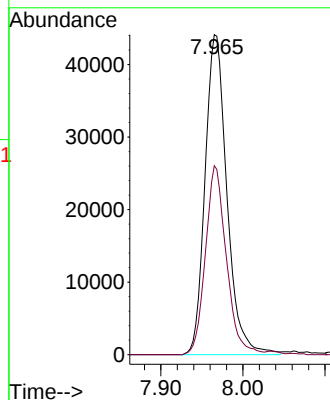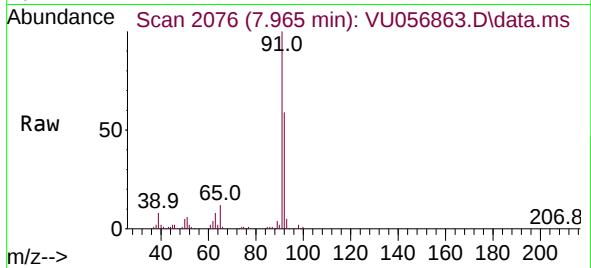

#48

2-Hexanone

Concen: 0.730 ug/L

RT: 8.688 min Scan# 2301

Delta R.T. 0.009 min

Lab File: VU056863.D

Acq: 15 Dec 2023 02:38

Tgt Ion: 43 Resp: 5245




Ion Ratio Lower Upper


43 100

58 29.1 47.5 71.3#

57 31.3 17.0 25.4#

100 10.4 9.8 14.8


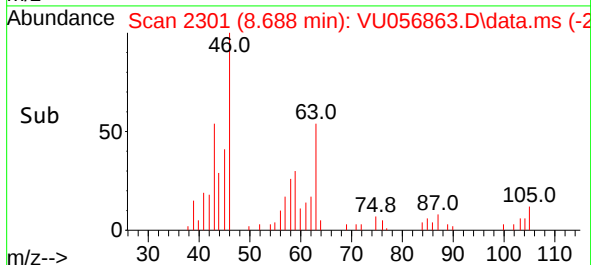
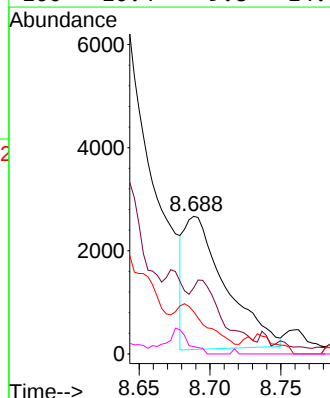
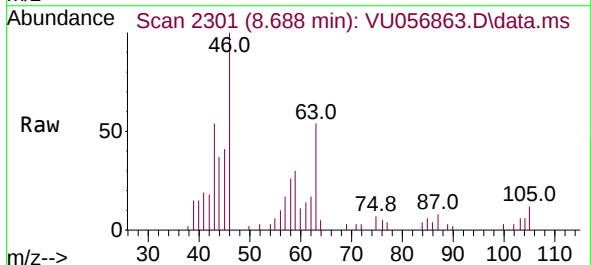


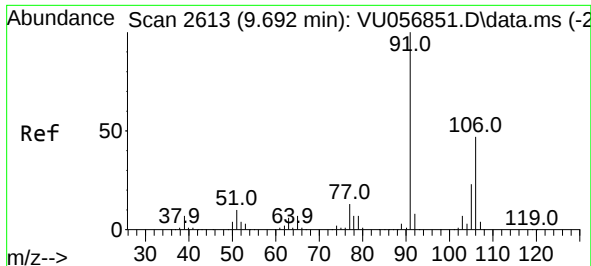

#53
m,p-Xylene
Concen: 0.166 ug/L
RT: 9.692 min Scan# 20
Delta R.T. -0.000 min
Lab File: VU056863.D
Acq: 15 Dec 2023 02:38




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:106 Resp: 5852
Ion Ratio Lower Upper
106 100
91 214.8 154.0 286.0

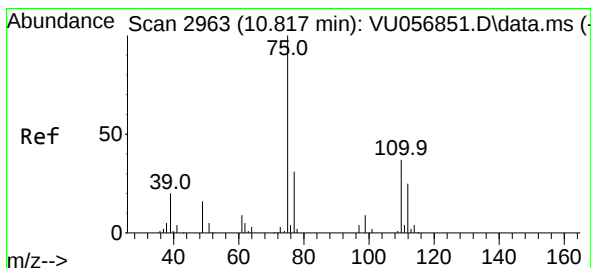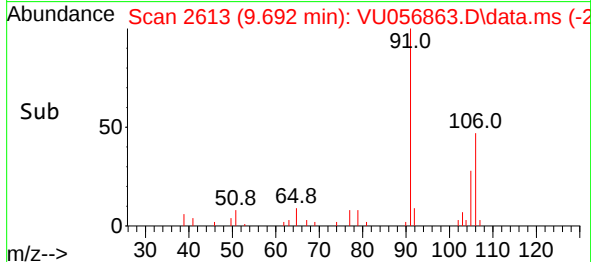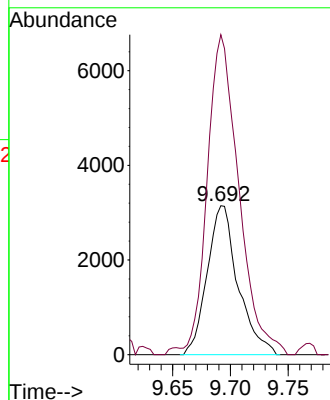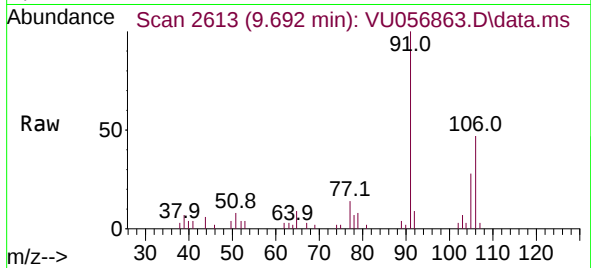

#61
1,2,3-Trichloropropane
Concen: 1.284 ug/L
RT: 11.807 min Scan# 3271
Delta R.T. 0.990 min
Lab File: VU056863.D
Acq: 15 Dec 2023 02:38

Tgt Ion: 75 Resp: 13557
Ion Ratio Lower Upper
75 100
110 1.4 28.4 42.6#
77 30.4 26.3 39.5

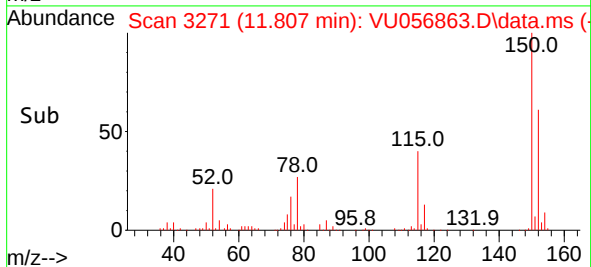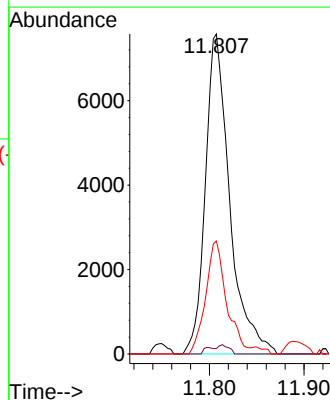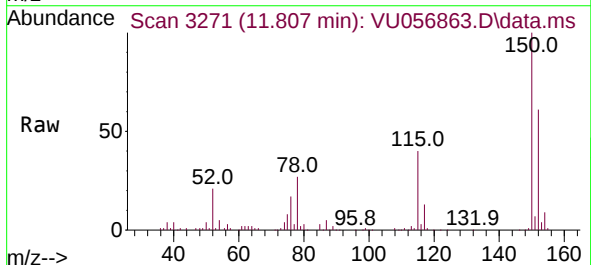

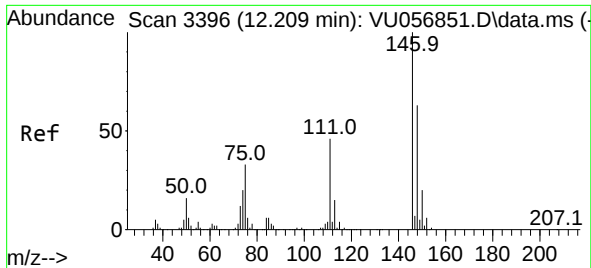

#67

1,2-Dichlorobenzene

Concen: 0.152 ug/L

RT: 12.209 min Scan# 31

Delta R.T. -0.000 min


Lab File: VU056863.D

Acq: 15 Dec 2023 02:38

Instrument :

MSVOA_U

ClientSampleId :

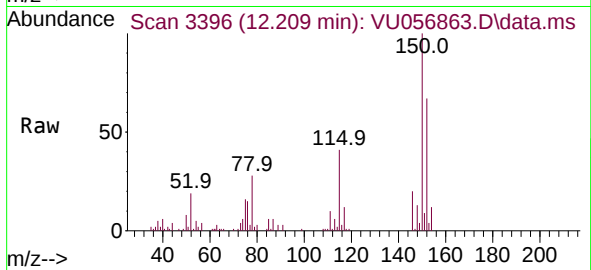

Tgt Ion:	146	Resp:	5100
Ion	Ratio	Lower	Upper
146	100		
111	51.5	36.9	55.3
148	65.8	53.0	79.4

