

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121423\
 Data File : VU056849.D
 Acq On : 14 Dec 2023 19:19
 Operator : MD/SY
 Sample : 05675-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AB8

Quant Time: Dec 15 00:55:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Dec 15 00:49:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	243263	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	249214	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	105109	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	66007	3.166	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	63.400%
7) Chloroethane-d5	1.907	69	57914	3.712	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	74.200%
11) 1,1-Dichloroethene-d2	2.560	65	30600	3.430	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.600%
20) 2-Butanone-d5	4.618	46	220142	53.460	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.920%
24) Chloroform-d	5.055	84	169735	4.299	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.000%
26) 1,2-Dichloroethane-d4	5.695	65	81762	4.376	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.600%
32) Benzene-d6	5.721	84	295504	3.823	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	76.400%
36) 1,2-Dichloropropane-d6	6.682	67	103416	4.274	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.400%
41) Toluene-d8	7.894	98	233824	3.384	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	67.600%#
43) trans-1,3-Dichloroprop...	8.174	79	36104	3.848	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.000%
46) 2-Hexanone-d5	8.631	63	169973	48.032	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.060%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	83484	4.769	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.400%
66) 1,2-Dichlorobenzene-d4	12.190	152	89566	4.335	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	86.600%
Target Compounds						Qvalue
12) 1,1-Dichloroethene	2.576	96	20401	1.033	ug/L	# 40
19) 1,1-Dichloroethane	3.862	63	16976	0.441	ug/L	91
22) cis-1,2-Dichloroethene	4.660	96	28291	1.299	ug/L	95
34) Trichloroethene	6.538	95	157345	6.549	ug/L	99
47) Tetrachloroethene	8.547	164	302400	17.985	ug/L	98
67) 1,2-Dichlorobenzene	12.203	146	7794	0.218	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121423\
Data File : VU056849.D
Acq On : 14 Dec 2023 19:19
Operator : MD/SY
Sample : 05675-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AB8

Quant Time: Dec 15 00:55:41 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Dec 15 00:49:12 2023
Response via : Initial Calibration




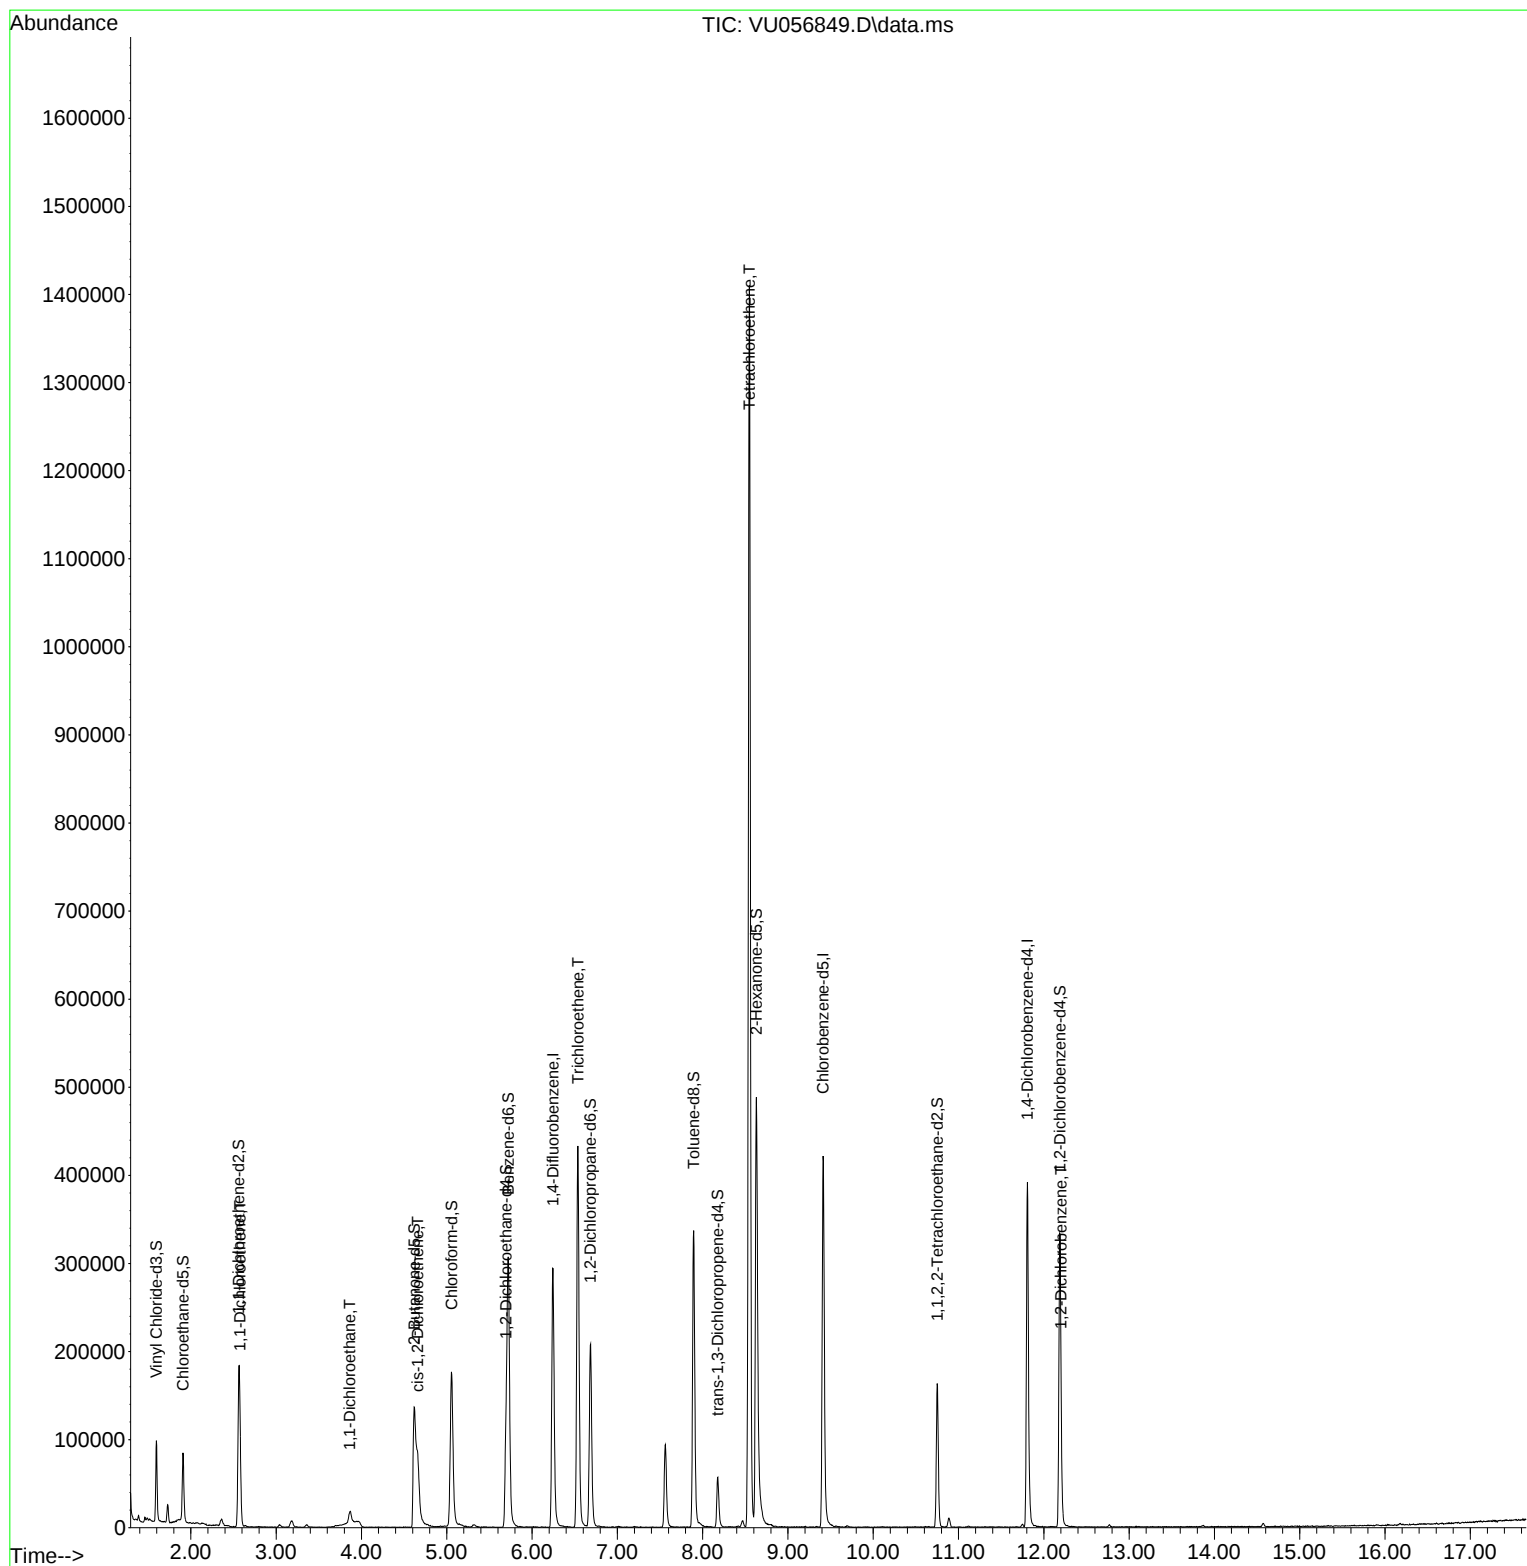


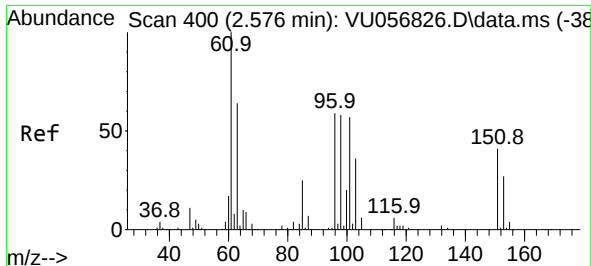

#12
1,1-Dichloroethene
Concen: 1.033 ug/L
RT: 2.576 min Scan# 400
Delta R.T. 0.000 min
Lab File: VU056849.D
Acq: 14 Dec 2023 19:19




Instrument :
MSVOA_U
ClientSampleId :
H0AB8


Tgt Ion: 96 Resp: 20401
Ion Ratio Lower Upper
96 100
61 193.3 119.0 221.0
63 262.8 88.7 164.7#

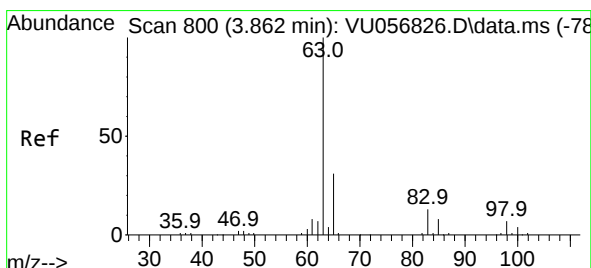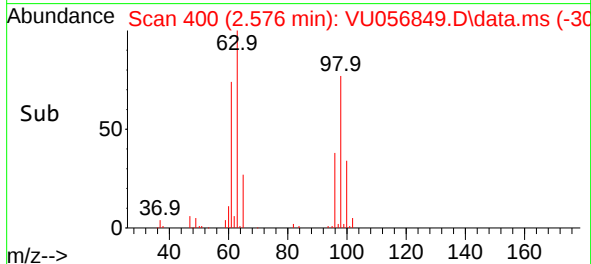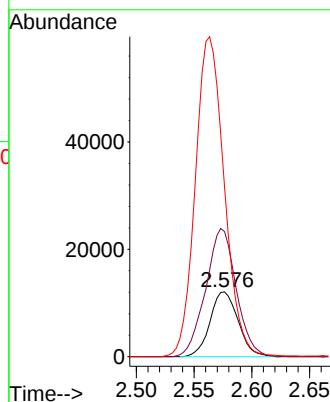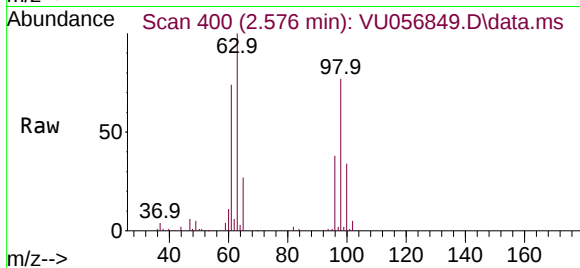

#19
1,1-Dichloroethane
Concen: 0.441 ug/L
RT: 3.862 min Scan# 800
Delta R.T. 0.000 min
Lab File: VU056849.D
Acq: 14 Dec 2023 19:19

Tgt Ion: 63 Resp: 16976
Ion Ratio Lower Upper
63 100
65 25.6 22.9 42.5
83 13.5 10.1 18.9


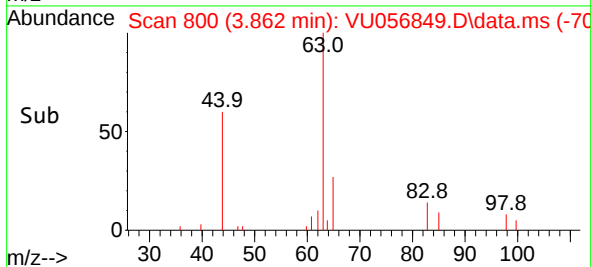
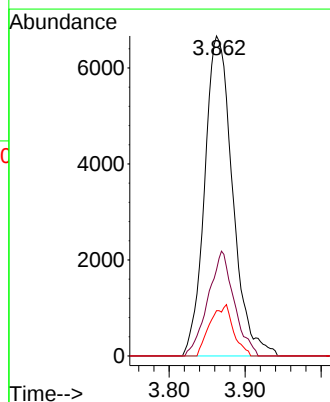
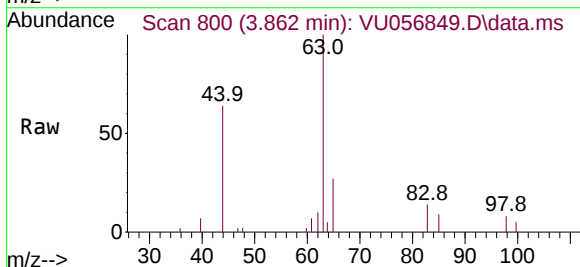


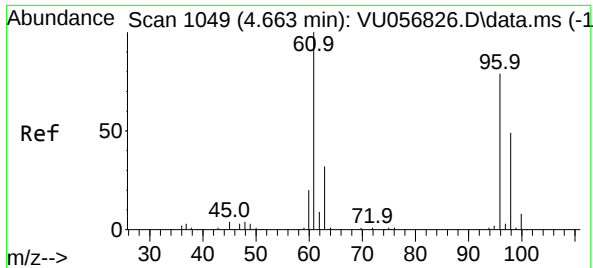

#22
 cis-1,2-Dichloroethene
 Concen: 1.299 ug/L
 RT: 4.660 min Scan# 1049
 Delta R.T. -0.003 min
 Lab File: VU056849.D
 Acq: 14 Dec 2023 19:19




Instrument :
 MSVOA_U
 ClientSampleId :
 H0AB8


Tgt Ion:	96	Resp:	28291
Ion	Ratio	Lower	Upper
96	100		
61	136.5	91.3	169.6
98	67.7	44.2	82.0

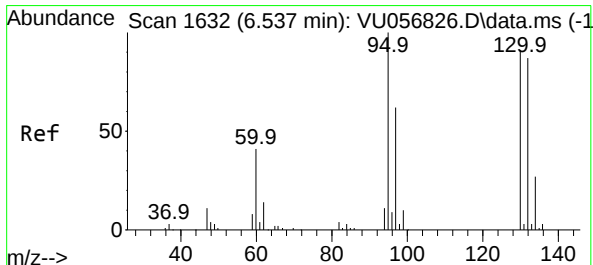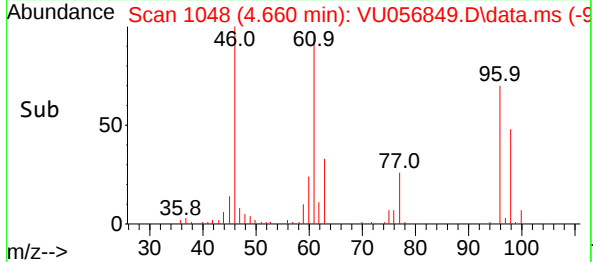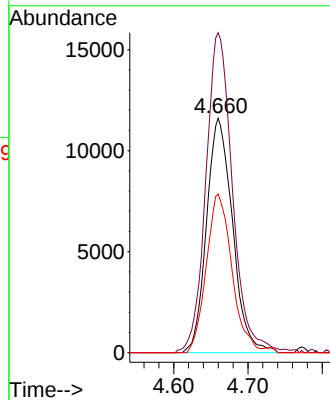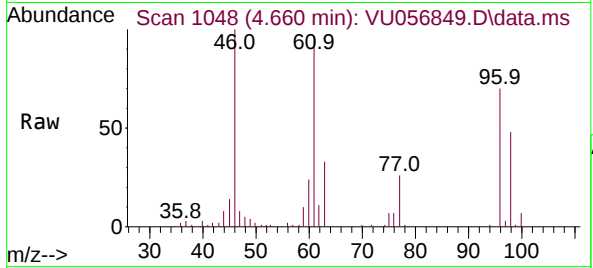

#34
 Trichloroethene
 Concen: 6.549 ug/L
 RT: 6.538 min Scan# 1632
 Delta R.T. 0.000 min
 Lab File: VU056849.D
 Acq: 14 Dec 2023 19:19

Tgt Ion:	95	Resp:	157345
Ion	Ratio	Lower	Upper
95	100		
97	64.1	46.1	85.5
132	90.2	63.6	118.0
130	93.1	66.4	123.4

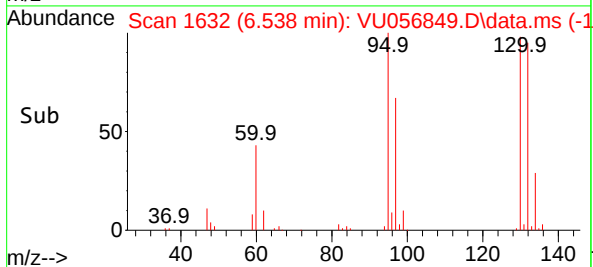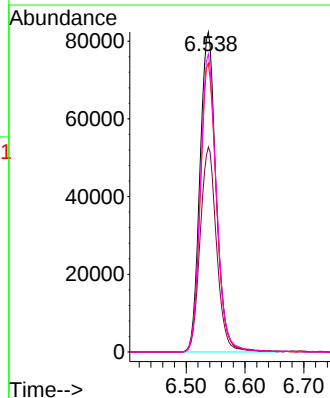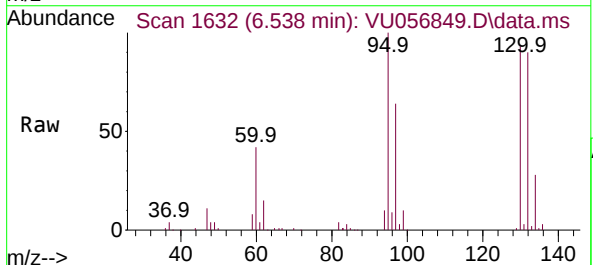




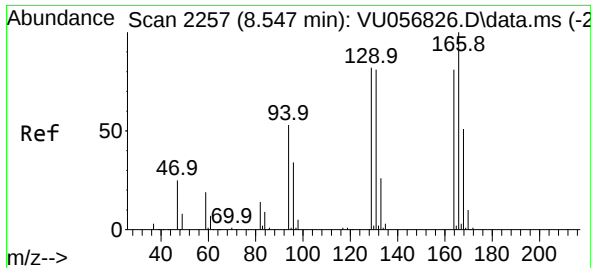


#47
Tetrachloroethene
Concen: 17.985 ug/L
RT: 8.547 min Scan# 21
Delta R.T. 0.000 min
Lab File: VU056849.D
Acq: 14 Dec 2023 19:19

Instrument :
MSVOA_U
ClientSampleId :
H0AB8

Tgt Ion:164 Resp: 302400

Ion	Ratio	Lower	Upper
164	100		
129	105.6	73.4	136.4
131	100.4	71.5	132.9
166	128.9	92.7	172.1

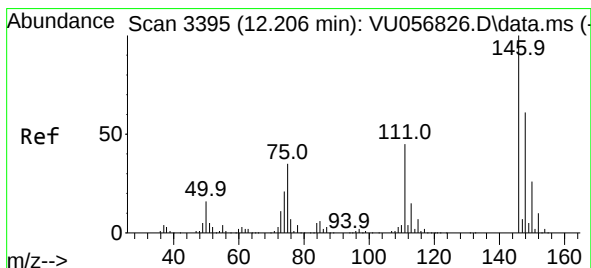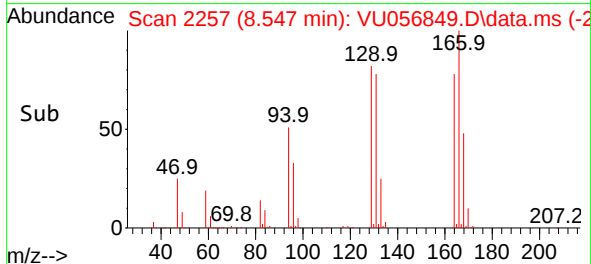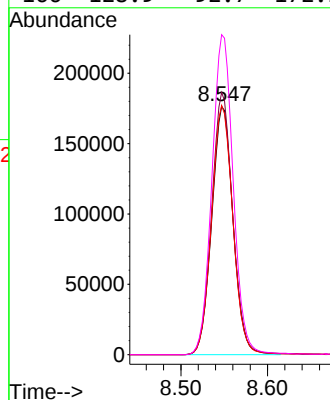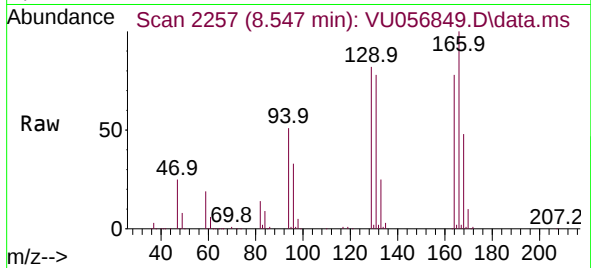

#67
1,2-Dichlorobenzene
Concen: 0.218 ug/L
RT: 12.203 min Scan# 3394
Delta R.T. -0.003 min
Lab File: VU056849.D
Acq: 14 Dec 2023 19:19

Tgt Ion:146 Resp: 7794

Ion	Ratio	Lower	Upper
146	100		
111	50.0	36.9	55.3
148	60.5	53.0	79.4

