

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121423\
 Data File : VU056854.D
 Acq On : 14 Dec 2023 23:01
 Operator : MD/SY
 Sample : 05731-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E0Y53

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU056854.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.387	25	30	36	rVB	16086	15813	1.65%	0.190%
2	1.580	82	90	107	rVV3	284940	458973	47.98%	5.525%
3	1.911	184	193	205	rBV	80846	109324	11.43%	1.316%
4	2.078	235	245	260	rBV	91346	135069	14.12%	1.626%
5	2.371	328	336	347	rBV2	11470	16472	1.72%	0.198%
6	2.563	382	396	412	rBV	147446	245058	25.62%	2.950%
7	3.178	576	587	613	rVB2	19665	47923	5.01%	0.577%
8	3.351	631	641	655	rBV5	8626	18028	1.88%	0.217%
9	4.657	1026	1047	1082	rBV3	242162	808879	84.56%	9.737%
10	5.059	1154	1172	1207	rVB	170069	422245	44.14%	5.083%
11	5.721	1358	1378	1389	rBV2	300443	809187	84.59%	9.741%
12	6.245	1528	1541	1576	rBV	278376	553453	57.86%	6.662%
13	6.563	1632	1640	1658	rVB9	6306	15497	1.62%	0.187%
14	6.685	1664	1678	1696	rBV	196657	393423	41.13%	4.736%
15	7.563	1939	1951	1969	rBV	91990	166629	17.42%	2.006%
16	7.792	2011	2022	2041	rBV3	28553	60230	6.30%	0.725%
17	7.894	2041	2054	2067	rVV	321321	578181	60.44%	6.960%
18	7.965	2068	2076	2097	rVB	87304	165783	17.33%	1.996%
19	8.177	2131	2142	2160	rBV2	54313	97328	10.17%	1.172%
20	8.631	2272	2283	2323	rBV2	453519	956577	100.00%	11.515%
21	9.415	2514	2527	2532	rBV	415424	740244	77.38%	8.911%
22	9.692	2599	2613	2627	rBV3	11180	22479	2.35%	0.271%
23	10.750	2931	2942	2960	rBV	159966	267453	27.96%	3.220%
24	11.807	3259	3271	3293	rBV	354575	631461	66.01%	7.601%
25	12.187	3377	3389	3409	rBV	322236	571524	59.75%	6.880%




Sum of corrected areas: 8307233

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121423\
Data File : VU056854.D
Acq On : 14 Dec 2023 23:01
Operator : MD/SY
Sample : 05731-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E0Y53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

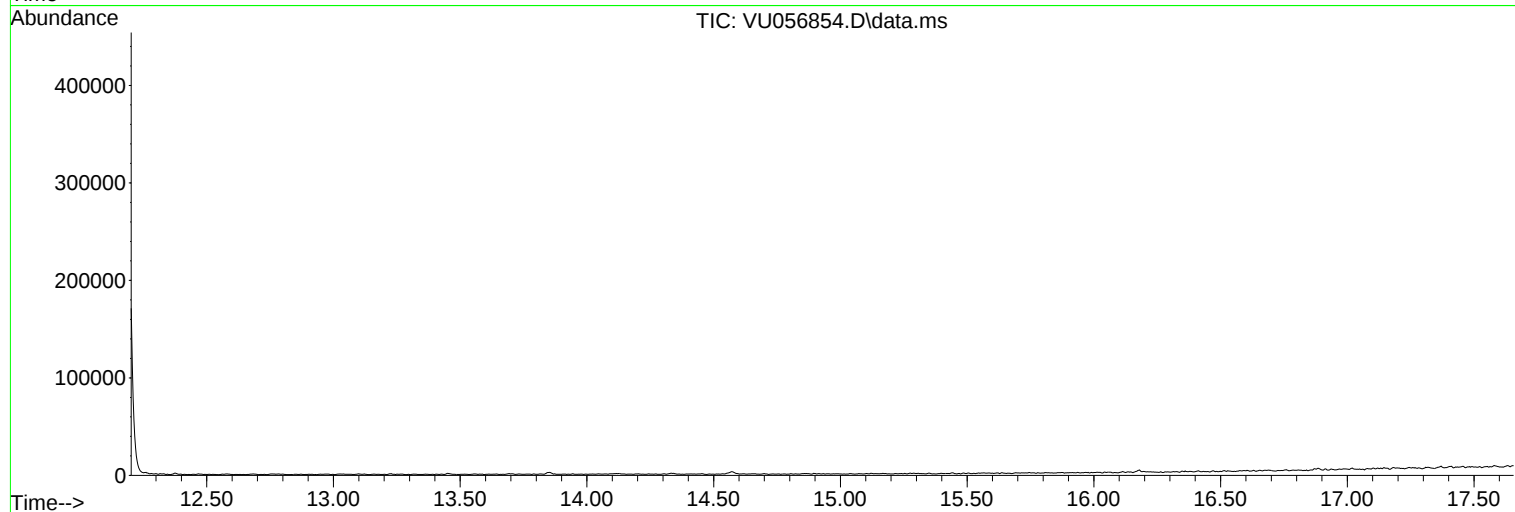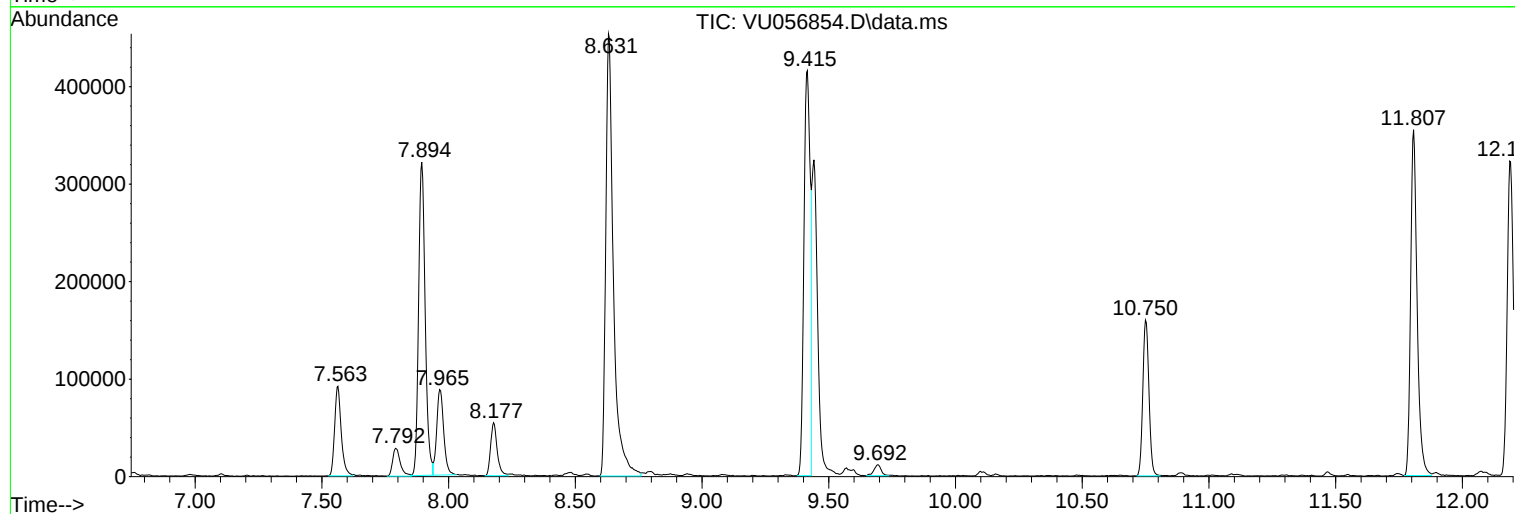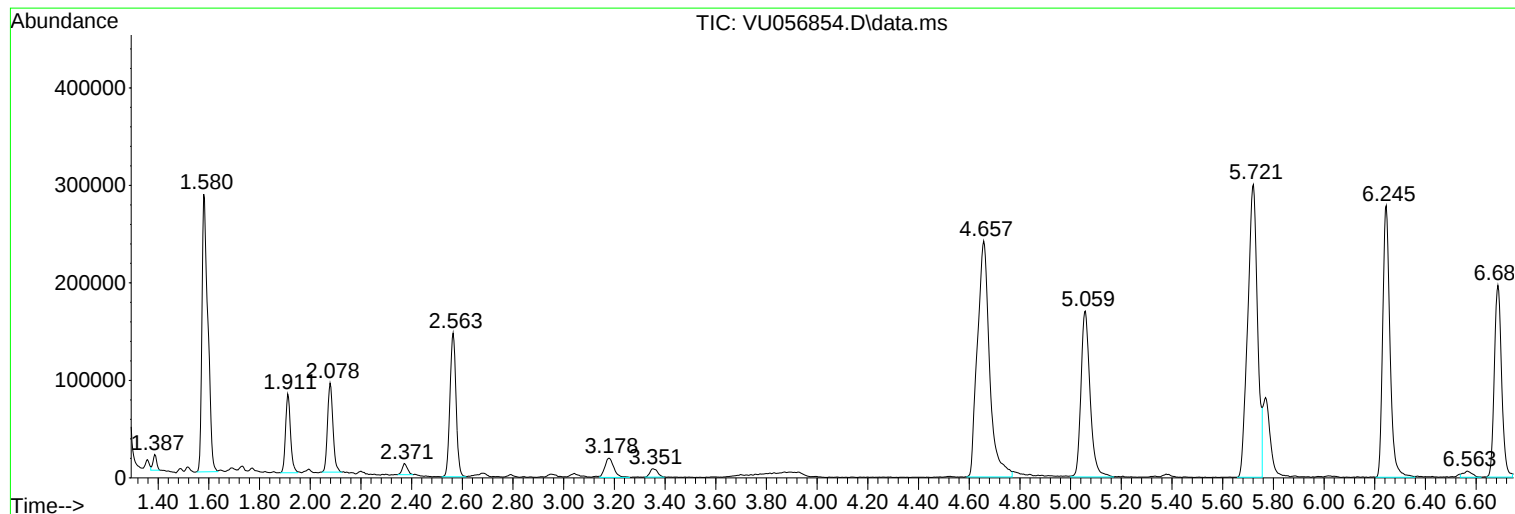

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121423\
Data File : VU056854.D
Acq On : 14 Dec 2023 23:01
Operator : MD/SY
Sample : 05731-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E0Y53










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Fluorodichloromethane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.078	1.22 ug/L	135069	1,4-Difluorobenzene	6.245

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
2			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
3			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
4			1-Hexyne	82	C6H10	000693-02-7	7
5			Methanamine, N,N-difluoro-	67	CH3F2N	000753-58-2	5

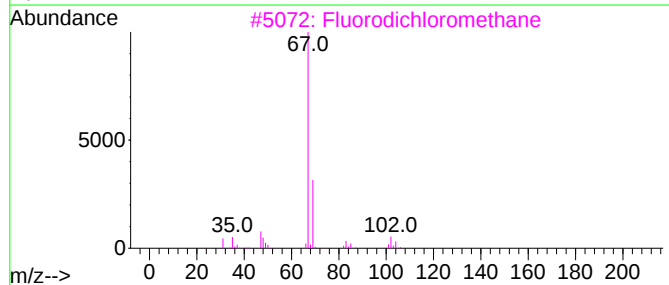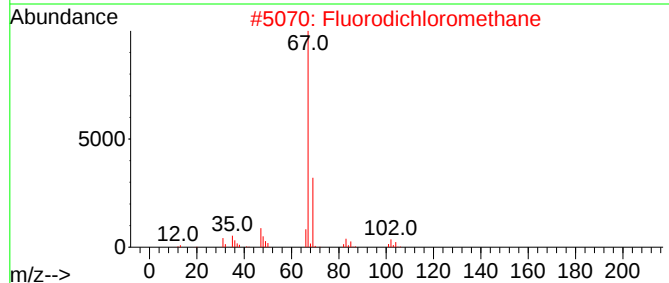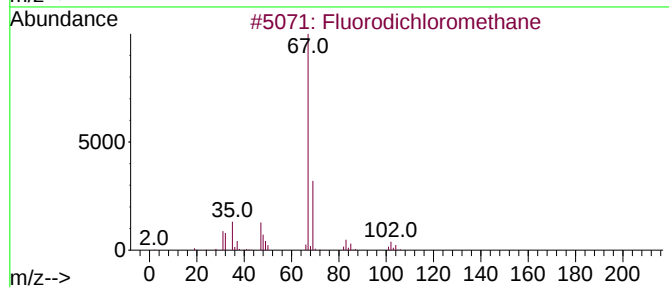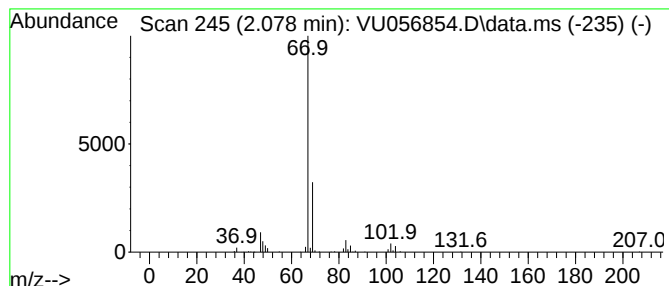

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121423\
Data File : VU056854.D
Acq On : 14 Dec 2023 23:01
Operator : MD/SY
Sample : 05731-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E0Y53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Fluorodichlorom...	2.078	1.2	ug/L	135069	1	6.245	553453	5.0