
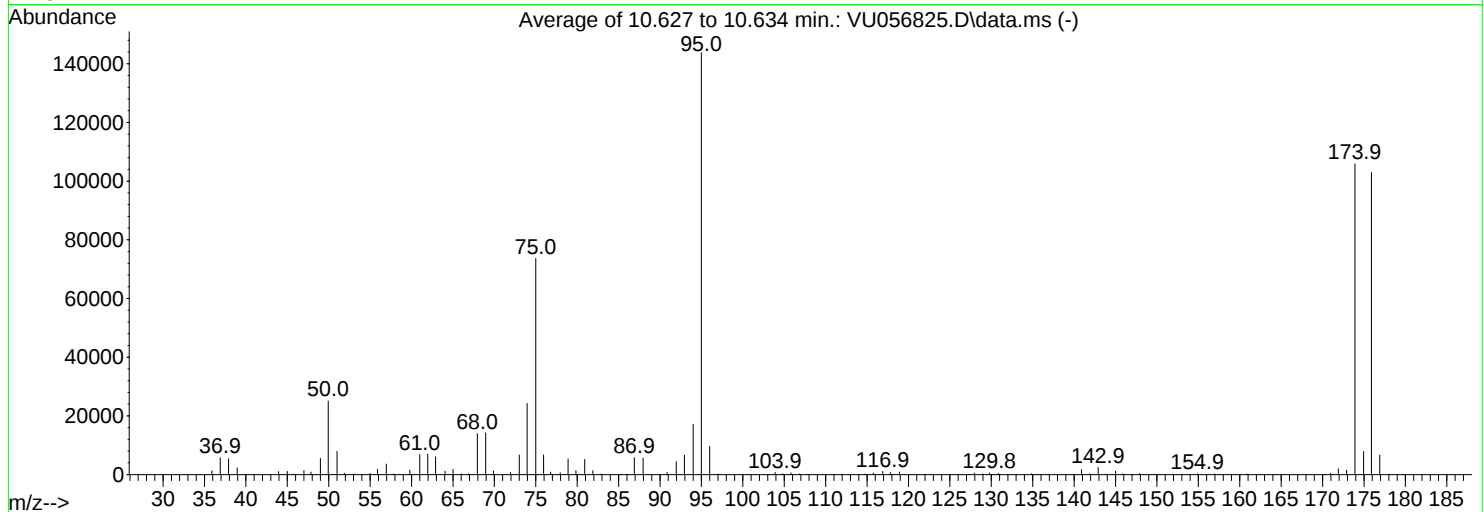


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121423\
Data File : VU056825.D
Acq On : 14 Dec 2023 08:59
Operator : MD/SY
Sample : BFB092
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB092

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Dec 18 01:16:15 2023

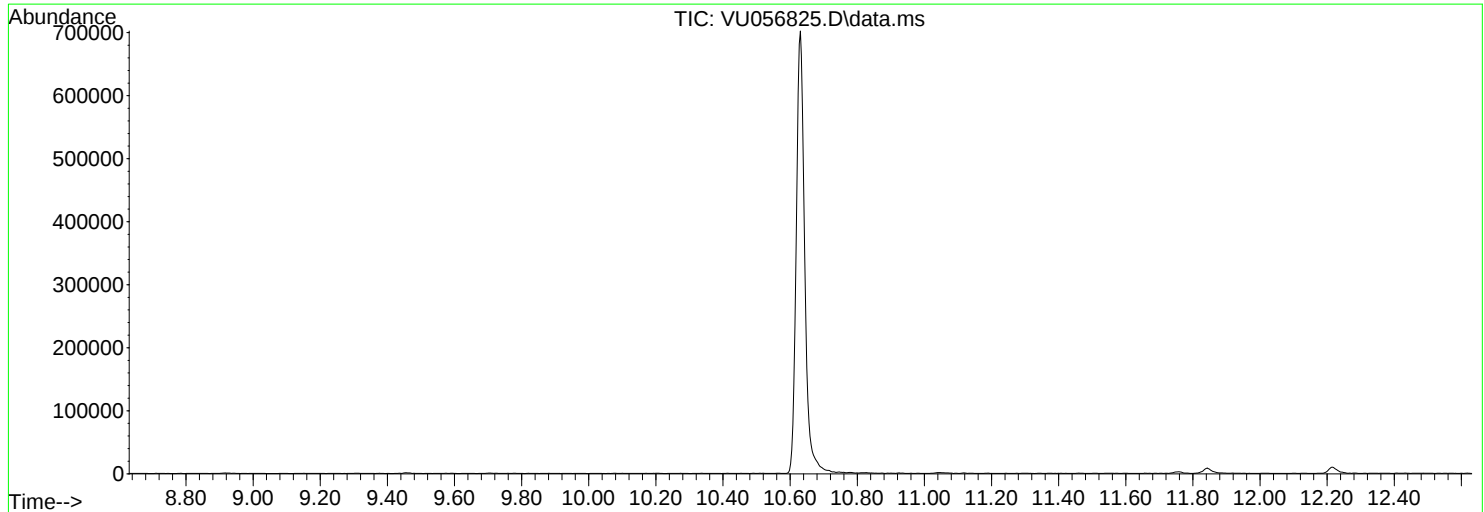

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	25075	PASS
75	95	30	80	51.3	73672	PASS
95	95	100	100	100.0	143744	PASS
96	95	5	9	6.7	9610	PASS
173	174	0.00	2	1.4	1509	PASS
174	95	50	120	73.7	105944	PASS
175	174	5	9	7.4	7810	PASS
176	174	95	101	97.1	102917	PASS
177	176	5	9	6.5	6698	PASS

m/z	Abundance
39.80	324.0
43.70	201.0
44.00	189.0

Instrument :
MSVOA_U
ClientSampleId :
BFB092

m/z	Abundance
35.90	1269.0
36.90	5887.0
37.90	5691.0
39.00	2389.0
40.00	519.0
40.90	159.0
43.90	1341.0
45.00	1188.0
45.80	192.0
47.00	1542.0
47.90	786.0
49.00	5656.0
49.90	25416.0
51.00	7954.0
51.90	384.0
53.10	173.0
55.10	382.0
55.90	1823.0
56.90	3795.0
58.00	128.0
59.80	1656.0
61.00	6515.0
62.00	7082.0
62.90	6226.0
64.00	1313.0
65.00	1720.0
66.00	264.0
66.90	324.0
68.00	14368.0
69.00	14360.0
69.90	1297.0
72.00	769.0
73.00	6615.0
74.00	25056.0
75.00	74416.0
75.90	6866.0
76.80	905.0
78.00	765.0
78.90	5204.0
79.80	1252.0
80.90	4987.0
81.90	1238.0
82.80	154.0
86.90	5950.0
88.00	5211.0
90.80	708.0
92.00	4922.0
93.00	6631.0
94.00	17192.0
95.00	144640.0
96.00	10276.0
97.10	224.0
103.90	739.0
104.80	246.0
105.80	704.0
106.80	172.0
107.70	131.0
111.90	114.0
112.80	150.0
114.70	233.0
115.70	545.0
116.90	1162.0
117.80	721.0
118.90	876.0
127.90	476.0
129.00	301.0
129.80	559.0
130.80	345.0
134.80	284.0
136.70	230.0
140.90	1569.0
141.90	295.0
142.90	2361.0
143.90	114.0
145.00	1172.0
145.90	292.0
147.90	339.0
149.60	123.0
151.90	128.0
154.90	322.0
156.90	227.0
159.00	130.0
160.80	205.0
171.00	339.0
171.90	1862.0
172.90	1425.0
173.90	102648.0
175.00	7875.0
175.90	100184.0
176.90	6540.0

Instrument :
MSVOA_U
ClientSampleId :
BFB092

m/z	Abundance
35.90	1301.0
36.90	5887.0
37.90	5500.0
39.00	2317.0
40.00	490.0
40.90	120.0
43.90	1262.0
45.00	1181.0
45.70	147.0
47.00	1401.0
47.80	865.0
49.00	5840.0
49.90	26096.0
51.00	8121.0
51.90	453.0
53.00	227.0
55.00	369.0
55.90	1862.0
57.00	3614.0
57.80	190.0
59.80	1642.0
61.00	7079.0
62.00	7067.0
62.90	6142.0
64.00	1223.0
65.00	1869.0
66.00	274.0
66.90	303.0
68.00	14358.0
68.90	14603.0
69.90	1316.0
71.20	108.0
72.00	772.0
73.00	6854.0
74.00	24832.0
75.00	75256.0
75.90	6964.0
76.80	912.0
77.90	669.0
78.90	5519.0
79.90	1415.0
80.90	5334.0
81.90	1361.0
82.80	137.0
86.90	5898.0
87.90	5762.0
90.80	753.0
92.00	4493.0
93.00	6782.0
94.00	17664.0
95.00	147904.0
96.00	9827.0
97.00	188.0
103.90	733.0
104.80	329.0
105.80	604.0
106.90	176.0
107.70	107.0
111.90	104.0
112.70	134.0
114.80	229.0
115.70	524.0
116.90	1110.0
117.80	714.0
118.90	889.0
127.90	500.0
129.00	291.0
129.80	638.0
130.80	373.0
134.90	298.0
136.90	203.0
140.90	1804.0
141.90	315.0
142.90	2538.0
143.90	171.0
145.00	1282.0
145.80	282.0
146.90	122.0
147.90	383.0
149.60	128.0
153.70	123.0
154.90	341.0
156.90	225.0
158.90	124.0
160.80	170.0
170.90	390.0
171.90	2044.0
172.90	1615.0
173.90	108912.0
174.90	8074.0
175.90	106224.0
176.90	6828.0

Instrument :
MSVOA_U
ClientSampleId :
BFB092

178.00

127.0

Instrument :
MSVOA_U
ClientSampleId :
BFB092

m/z	Abundance
35.90	1259.0
36.90	5310.0
37.90	4878.0
38.90	2143.0
40.00	404.0
44.00	1071.0
45.00	1042.0
47.00	1198.0
47.80	828.0
49.00	5191.0
50.00	23712.0
51.00	7750.0
51.90	407.0
53.00	279.0
53.90	123.0
54.90	419.0
55.90	1845.0
57.00	3328.0
57.80	202.0
59.80	1378.0
61.00	6840.0
61.90	6587.0
62.90	5639.0
64.10	1060.0
65.00	1772.0
66.10	219.0
66.90	317.0
67.90	13120.0
68.90	13737.0
69.90	1146.0
71.90	710.0
73.00	6563.0
73.90	22856.0
75.00	71344.0
76.00	6249.0
76.80	793.0
77.90	479.0
78.90	5349.0
79.90	1493.0
80.90	5212.0
81.90	1342.0
82.80	140.0
86.90	5339.0
87.90	5775.0
90.90	684.0
91.90	3704.0
92.90	6502.0
94.00	16632.0
95.00	138688.0
96.00	8728.0
97.00	196.0
102.80	105.0
103.90	667.0
104.80	354.0
105.80	484.0
106.90	168.0
110.90	108.0
114.80	204.0
115.80	496.0
116.90	996.0
117.80	603.0
118.90	854.0
128.00	521.0
128.90	220.0
129.80	600.0
130.90	327.0
134.90	343.0
137.00	223.0
139.90	135.0
140.90	1694.0
141.90	287.0
142.90	2323.0
143.80	183.0
145.00	1166.0
145.80	204.0
146.90	118.0
147.90	353.0
153.70	127.0
154.90	333.0
156.90	219.0
158.90	133.0
160.90	134.0
170.90	441.0
171.90	2002.0
172.90	1486.0
173.90	106272.0
174.90	7481.0
175.90	102344.0
176.90	6727.0
178.00	212.0

Instrument :
MSVOA_U
ClientSampleId :
BFB092