

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121624\
 Data File : VU062347.D
 Acq On : 16 Dec 2024 16:26
 Operator : MD/SY
 Sample : P5269-06
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7J55

Quant Time: Dec 17 00:35:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Dec 17 00:31:28 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		6.242	114	87799	5.000	ug/L	0.00
28) Chlorobenzene-d5		9.412	117	81998	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.804	152	36721	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.596	65	32859	5.548	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	111.000%	
7) Chloroethane-d5		1.908	69	25154	5.971	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	119.400%	
11) 1,1-Dichloroethene-d2		2.560	65	15832	5.619	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	112.400%	
20) 2-Butanone-d5		4.621	46	64402	56.744	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.480%	
24) Chloroform-d		5.052	84	72577	5.663	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	113.200%	
26) 1,2-Dichloroethane-d4		5.692	65	38924	6.176	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	123.600%	
32) Benzene-d6		5.718	84	133006	5.632	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	112.600%	
36) 1,2-Dichloropropane-d6		6.682	67	38949	5.764	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	115.200%	
41) Toluene-d8		7.891	98	122353	5.484	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.600%	
43) trans-1,3-Dichloroprop...		8.174	79	15991	5.376	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	107.600%	
46) 2-Hexanone-d5		8.628	63	49536	55.204	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	110.400%	
56) 1,1,2,2-Tetrachloroeth...		10.746	84	30450	5.791	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	115.800%	
66) 1,2-Dichlorobenzene-d4		12.184	152	43443	6.420	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	128.400%#	
Target Compounds							
13) Acetone		2.641	43	9778	12.653	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121624\
Data File : VU062347.D
Acq On : 16 Dec 2024 16:26
Operator : MD/SY
Sample : P5269-06
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7J55

Quant Time: Dec 17 00:35:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Dec 17 00:31:28 2024
Response via : Initial Calibration

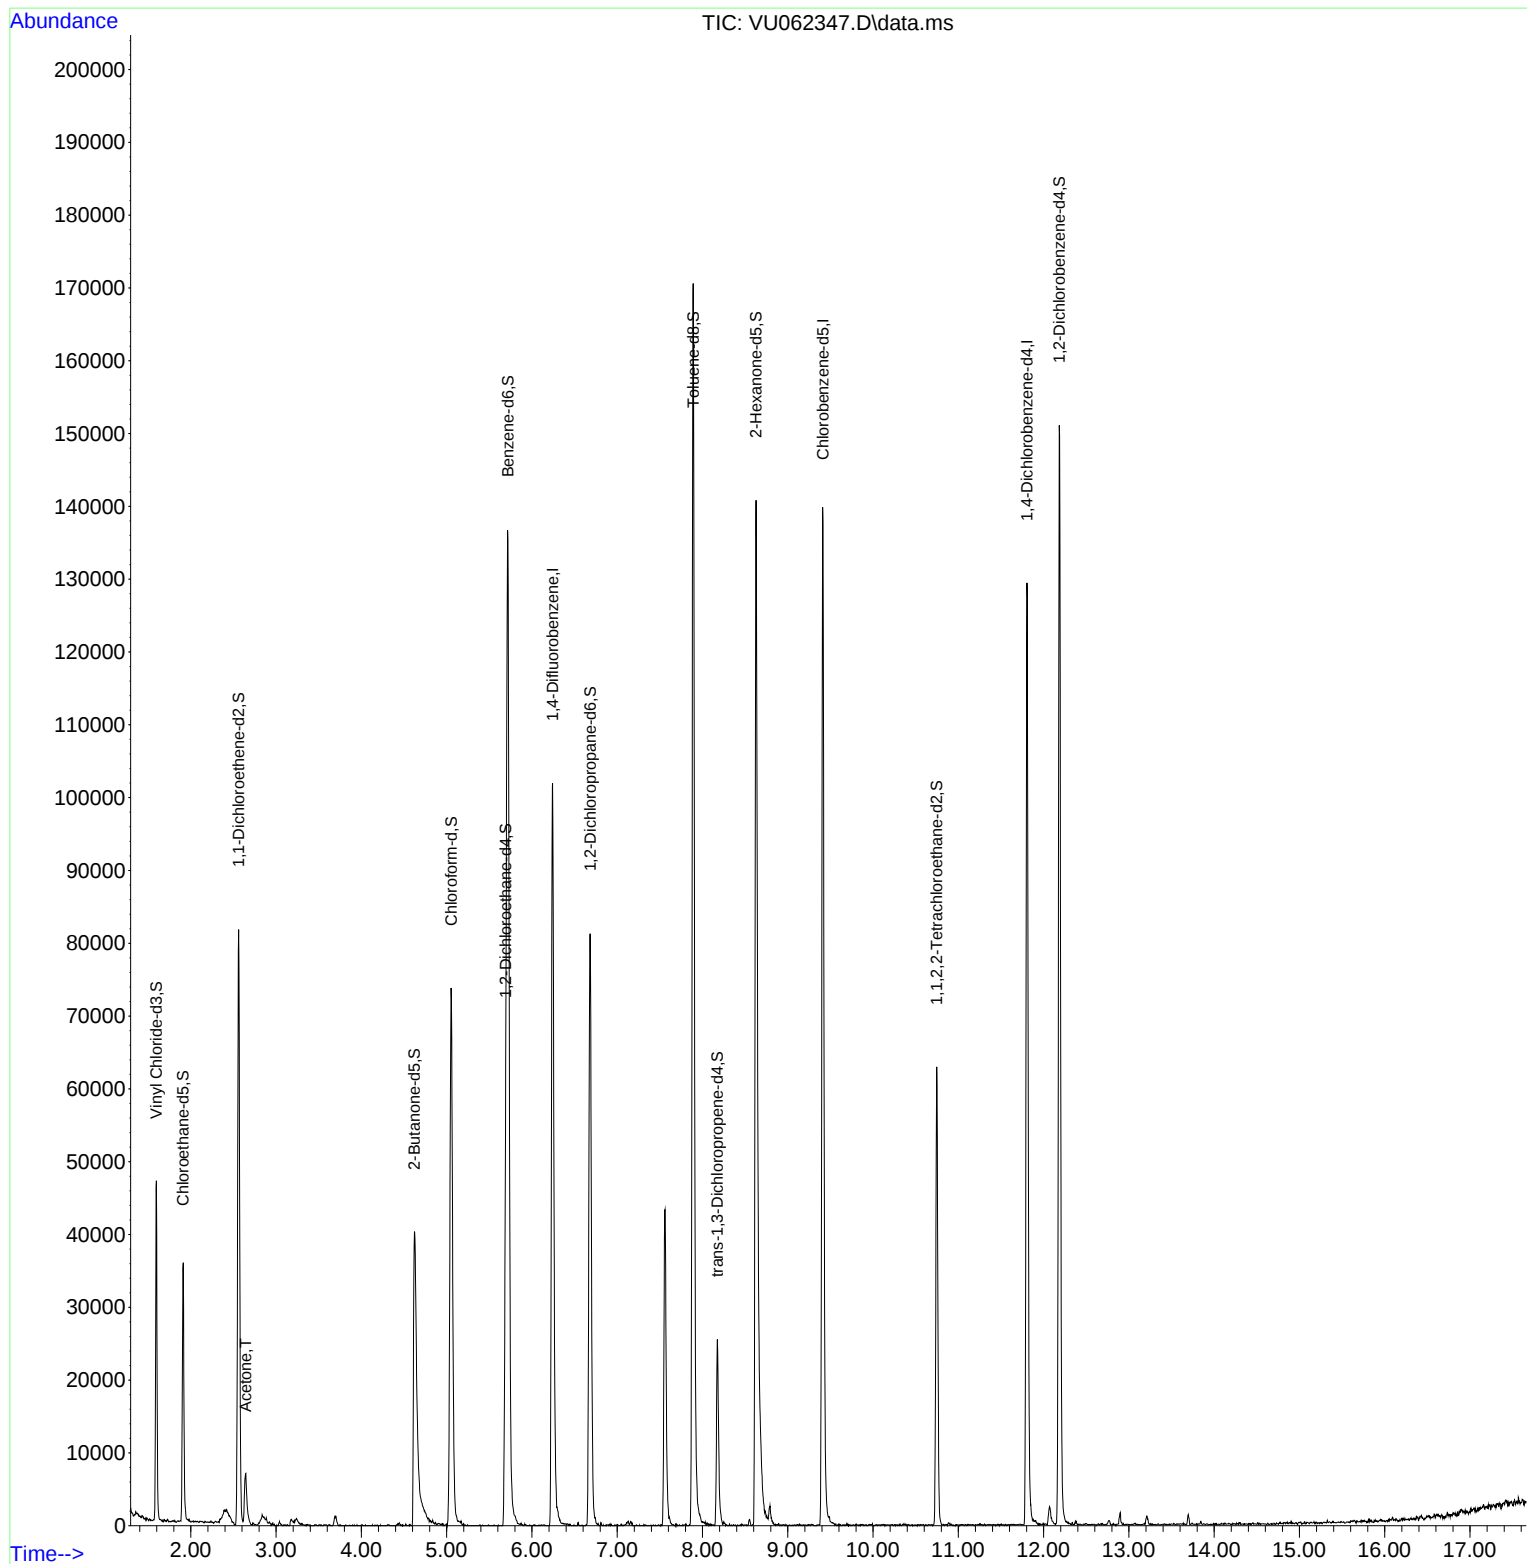

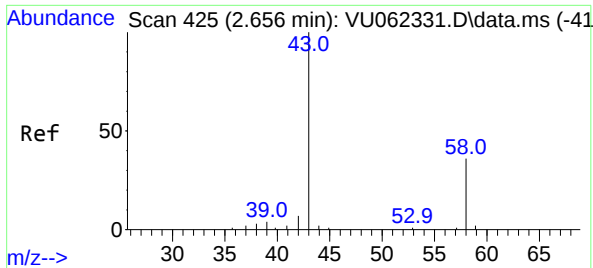

Acetone
 Concen: 12.653 ug/L
 RT: 2.641 min Scan# 41
 Delta R.T. -0.016 min
 Lab File: VU062347.D
 Acq: 16 Dec 2024 16:26

Instrument : MSVOA_U
 ClientSampleId : F7J55

Tgt Ion: 43 Resp: 9778

Ion	Ratio	Lower	Upper
43	100		
58	33.0	0.0	64.0

