

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121624\
 Data File : VU062358.D
 Acq On : 17 Dec 2024 00:43
 Operator : MD/SY
 Sample : P5262-04DL 50X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E2AW1DL

Quant Time: Dec 17 01:29:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Dec 17 01:28:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	97235	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	93875	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	42643	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	32407	4.941	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.800%
7) Chloroethane-d5	1.908	69	24568	5.266	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.400%
11) 1,1-Dichloroethene-d2	2.560	65	16001	5.128	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	102.600%
20) 2-Butanone-d5	4.628	46	60802	48.373	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.740%
24) Chloroform-d	5.052	84	69744	4.913	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.200%
26) 1,2-Dichloroethane-d4	5.692	65	37837	5.421	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.400%
32) Benzene-d6	5.718	84	128054	4.736	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.800%
36) 1,2-Dichloropropane-d6	6.682	67	36768	4.753	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.000%
41) Toluene-d8	7.891	98	117759	4.611	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.200%
43) trans-1,3-Dichloroprop...	8.177	79	15005	4.407	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.200%
46) 2-Hexanone-d5	8.628	63	43215	42.067	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.140%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	28127	4.672	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.400%
66) 1,2-Dichlorobenzene-d4	12.187	152	42064	5.353	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.000%
Target Compounds						
					Qvalue	
47) Tetrachloroethene	8.547	164	36662	5.762	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121624\
Data File : VU062358.D
Acq On : 17 Dec 2024 00:43
Operator : MD/SY
Sample : P5262-04DL 50X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E2AW1DL

Quant Time: Dec 17 01:29:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Dec 17 01:28:58 2024
Response via : Initial Calibration

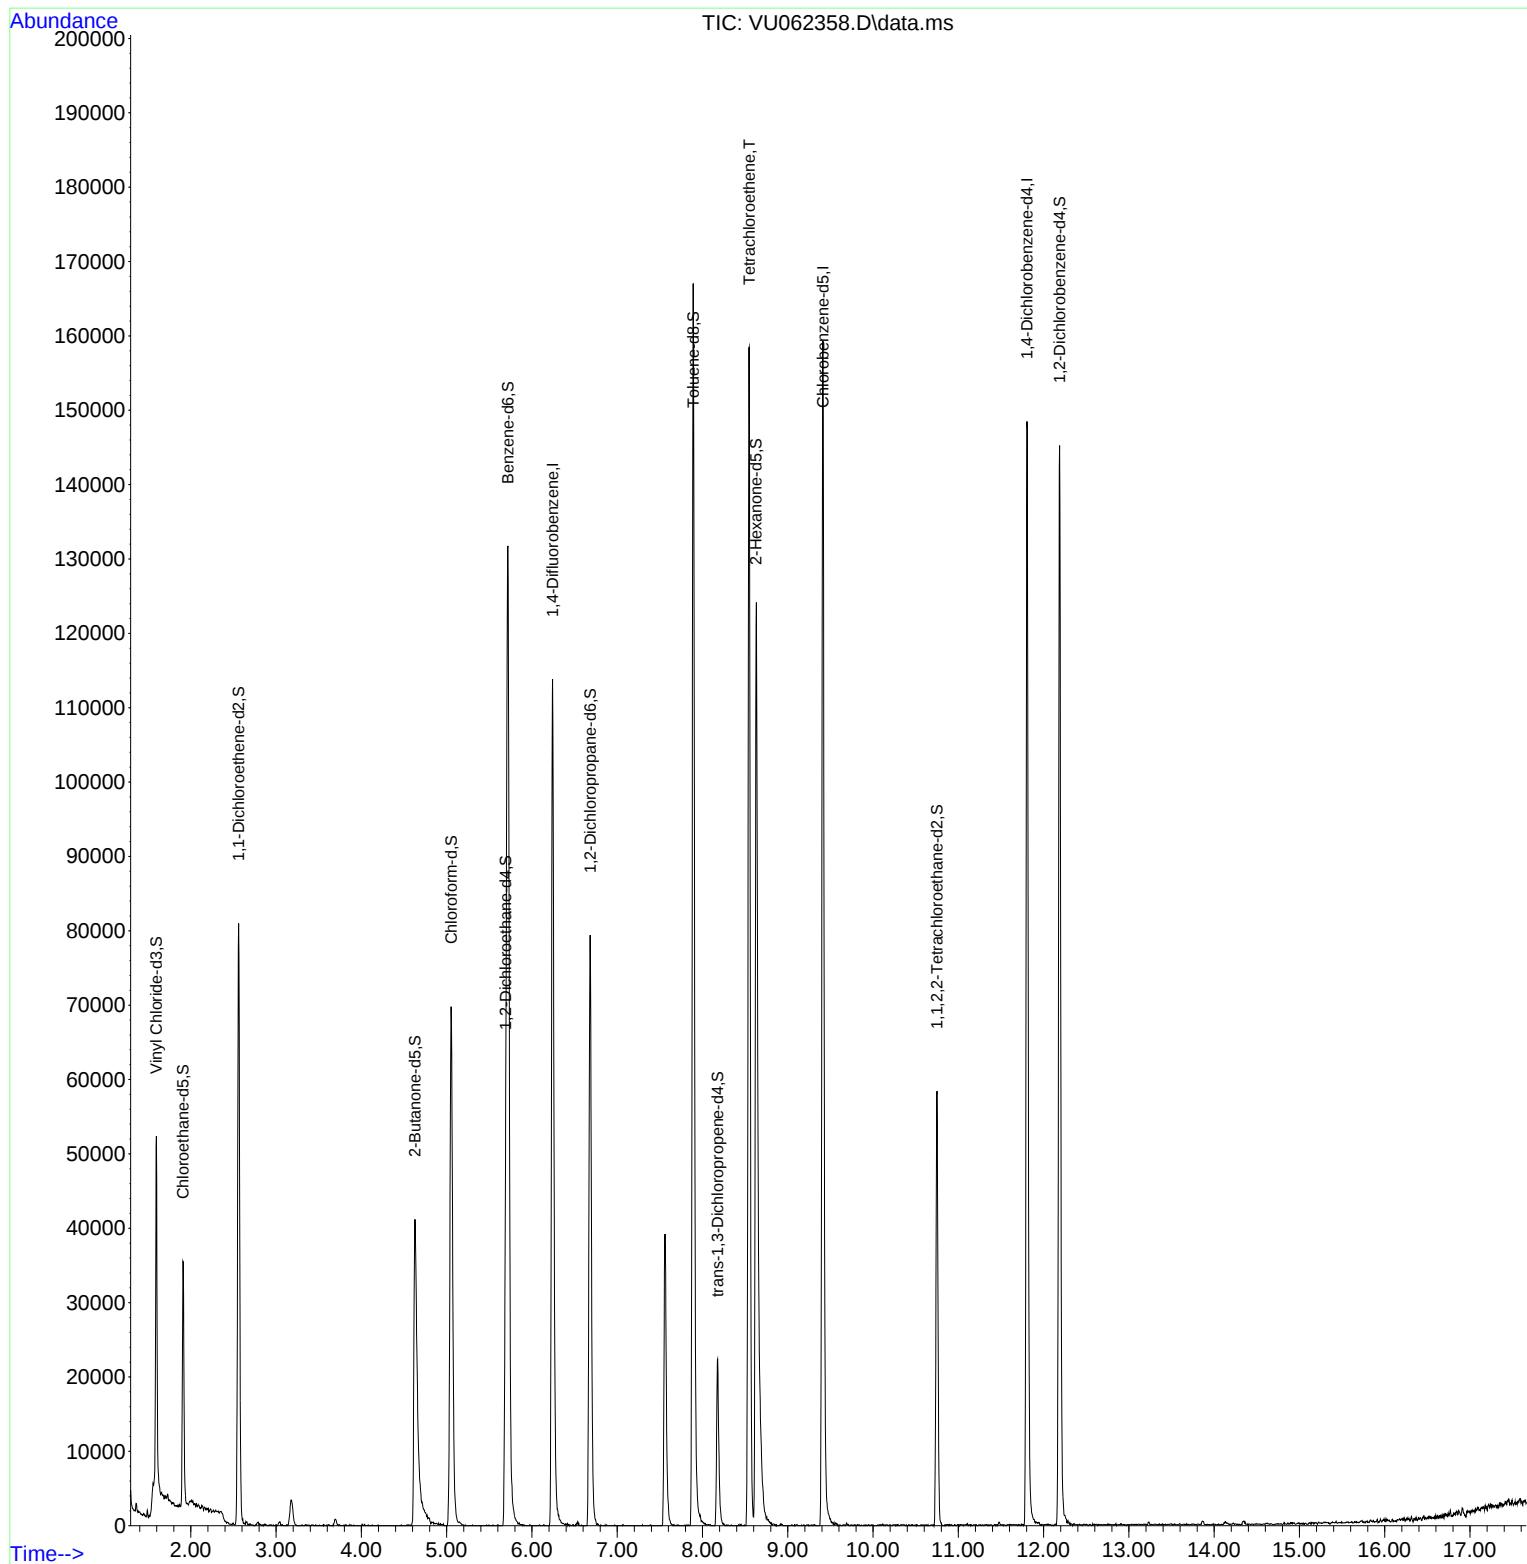

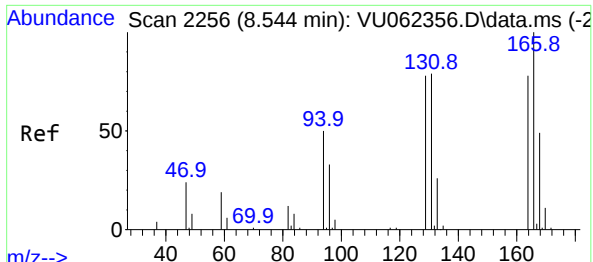

#47
Tetrachloroethene
Concen: 5.762 ug/L
RT: 8.547 min Scan# 21
Delta R.T. 0.004 min
Lab File: VU062358.D
Acq: 17 Dec 2024 00:43

Instrument :
MSVOA_U
ClientSampleId :
E2AW1DL

Tgt Ion:164 Resp: 36662

Ion	Ratio	Lower	Upper
164	100		
129	99.4	73.2	136.0
131	95.1	72.3	134.3
166	128.6	90.2	167.4

