

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121624\
 Data File : VU062364.D
 Acq On : 17 Dec 2024 03:10
 Operator : MD/SY
 Sample : P5274-06DL 5X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH8B5DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU062364.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	86	95	106	rBV	40717	48349	8.73%	1.304%
2	1.907	184	192	206	rBV	30877	41238	7.45%	1.112%
3	2.557	382	394	411	rBV	73321	119355	21.56%	3.219%
4	3.177	573	587	606	rVB	11051	25371	4.58%	0.684%
5	4.634	1025	1040	1073	rBV3	46381	157055	28.37%	4.236%
6	5.052	1154	1170	1193	rBV	68600	158927	28.71%	4.287%
7	5.714	1358	1376	1407	rBV2	125609	330173	59.65%	8.906%
8	6.238	1528	1539	1564	rBV	105726	202820	36.64%	5.471%
9	6.531	1618	1630	1665	rBV	225008	430313	77.74%	11.607%
10	6.679	1665	1676	1702	rVB2	75617	149688	27.04%	4.038%
11	7.557	1939	1949	1967	rBV	36747	67630	12.22%	1.824%
12	7.891	2039	2053	2075	rBV	152844	274945	49.67%	7.416%
13	8.174	2130	2141	2157	rBV2	22442	39283	7.10%	1.060%
14	8.544	2244	2256	2273	rBV	324817	553518	100.00%	14.930%
15	8.630	2273	2283	2323	rVB2	134227	293303	52.99%	7.911%
16	9.409	2514	2525	2548	rBV	142727	250945	45.34%	6.769%
17	10.746	2929	2941	2961	rBB	60424	98197	17.74%	2.649%
18	11.804	3259	3270	3292	rBV	134146	226175	40.86%	6.101%
19	12.187	3376	3389	3412	rBV	141403	240024	43.36%	6.474%




Sum of corrected areas: 3707309

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121624\
Data File : VU062364.D
Acq On : 17 Dec 2024 03:10
Operator : MD/SY
Sample : P5274-06DL 5X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH8B5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

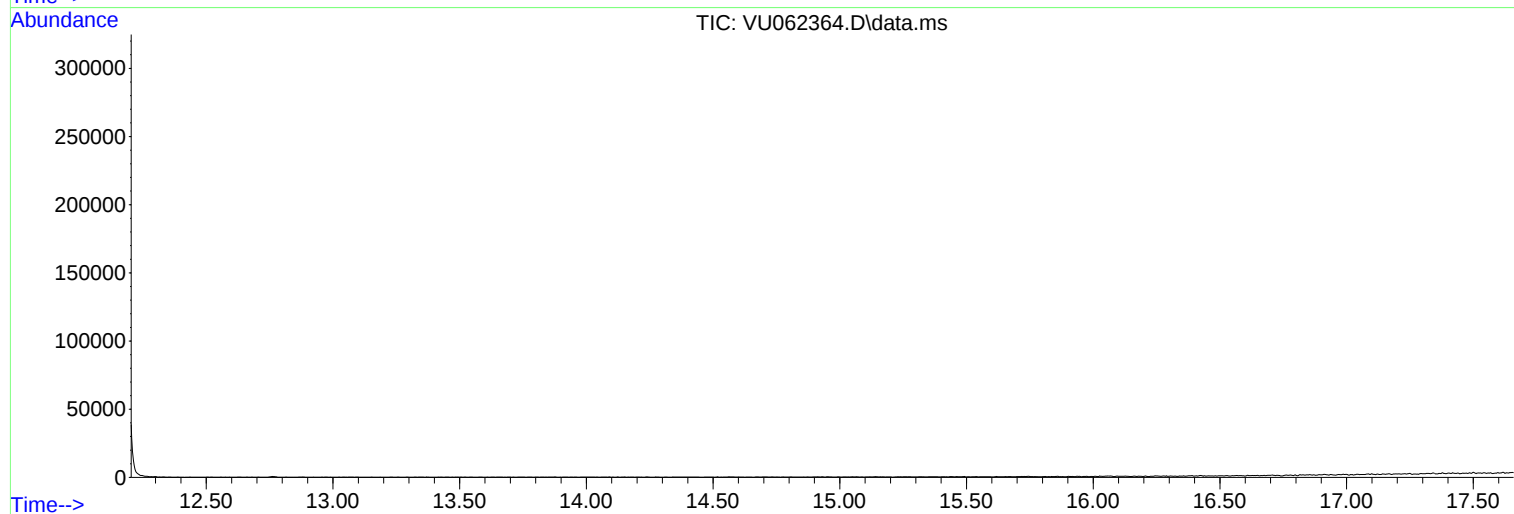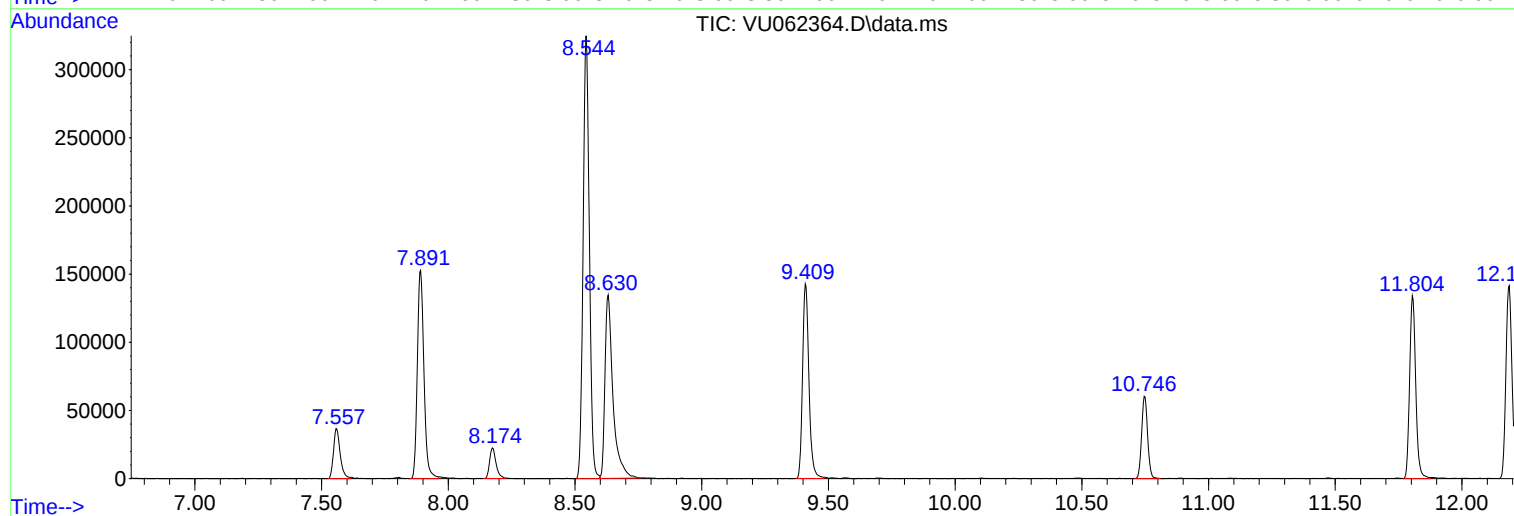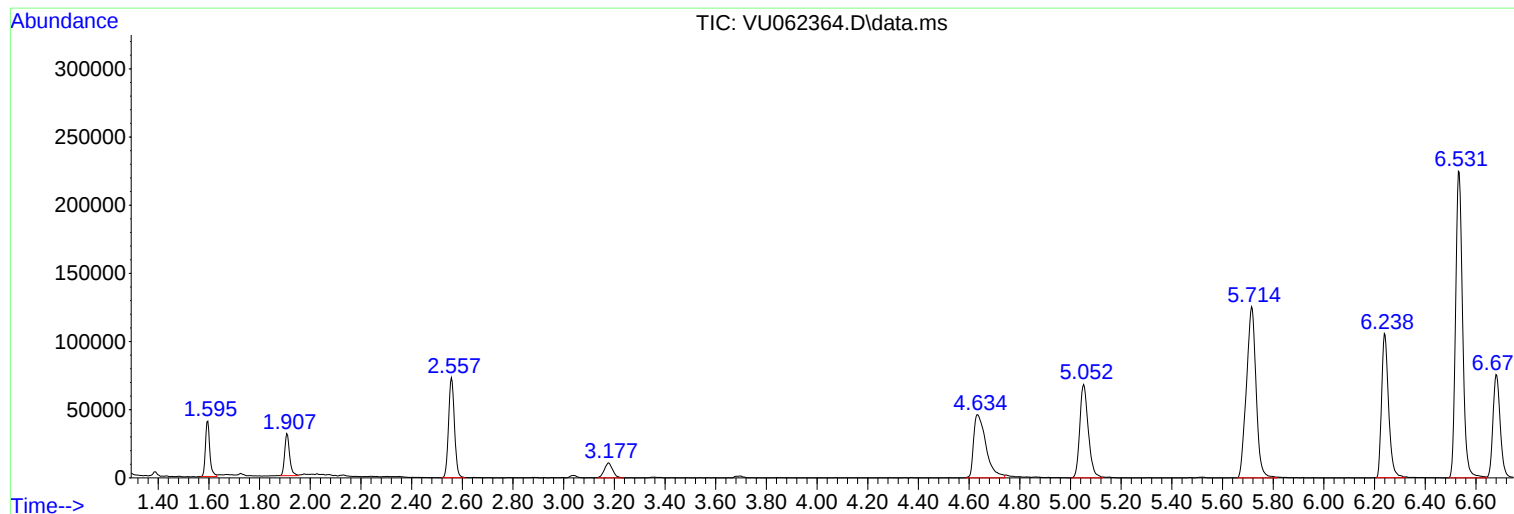

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121624\
Data File : VU062364.D
Acq On : 17 Dec 2024 03:10
Operator : MD/SY
Sample : P5274-06DL 5X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH8B5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121624\
Data File : VU062364.D
Acq On : 17 Dec 2024 03:10
Operator : MD/SY
Sample : P5274-06DL 5X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH8B5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc