


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121624\
Data File : VU062330.D
Acq On : 16 Dec 2024 08:14
Operator : MD/SY
Sample : BFB047
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB047

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Dec 18 01:12:26 2024

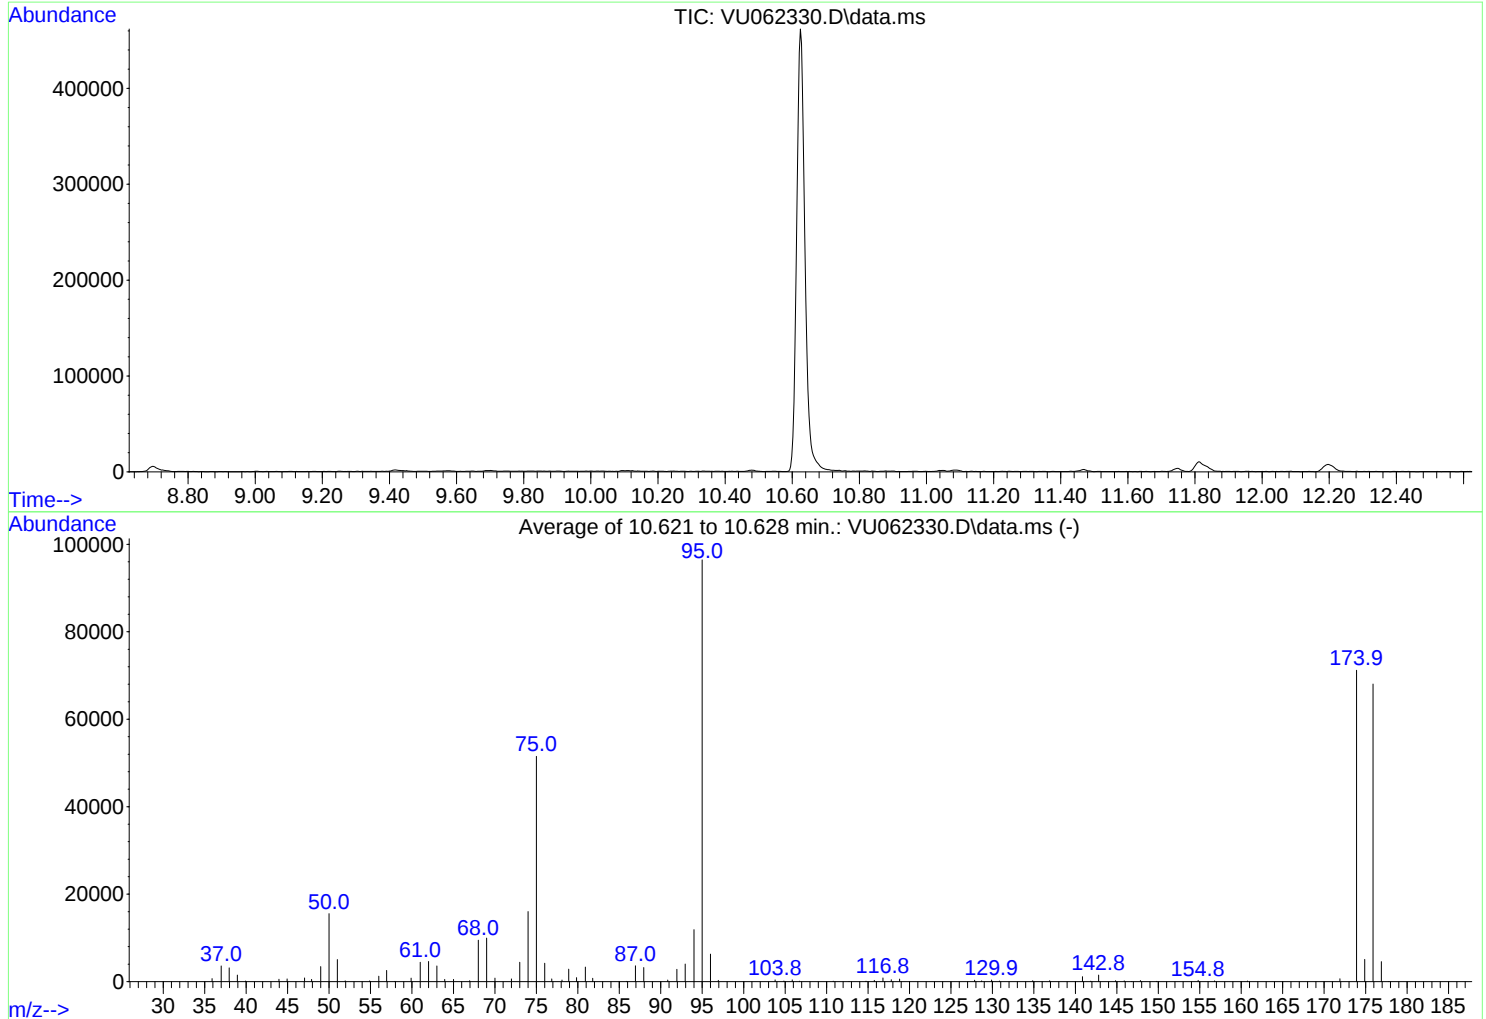

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2889

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.1	15557	PASS
75	95	30	80	53.4	51528	PASS
95	95	100	100	100.0	96443	PASS
96	95	5	9	6.5	6289	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.8	71205	PASS
175	174	5	9	7.1	5082	PASS
176	174	95	101	95.6	68048	PASS
177	176	5	9	6.7	4578	PASS

m/z	Abundance
36.00	283.0
37.90	118.0

Instrument :
MSVOA_U
ClientSampleId :
BFB047

m/z	Abundance
35.90	974.0
37.00	3535.0
38.00	3231.0
38.90	1453.0
39.90	103.0
44.00	507.0
45.00	651.0
47.00	897.0
47.90	502.0
49.00	3498.0
50.00	15743.0
51.00	5047.0
52.00	171.0
54.90	150.0
56.00	1222.0
56.90	2541.0
57.90	115.0
59.90	754.0
61.00	4448.0
62.00	4648.0
63.00	3580.0
64.00	501.0
65.00	595.0
66.90	252.0
68.00	9520.0
69.00	9664.0
70.00	707.0
72.00	645.0
73.00	4189.0
74.00	15772.0
75.00	50576.0
76.00	4109.0
76.90	590.0
78.10	411.0
78.90	2865.0
79.90	961.0
80.90	3311.0
81.80	799.0
86.90	3402.0
87.90	3164.0
90.90	369.0
92.00	2742.0
93.00	4054.0
94.00	11661.0
95.00	94072.0
96.00	6325.0
97.10	270.0
103.80	412.0
104.80	139.0
105.80	400.0
106.80	116.0
110.80	105.0
112.70	105.0
114.70	109.0
115.80	281.0
116.80	839.0
117.80	378.0
118.80	575.0
127.80	316.0
128.70	153.0
129.90	356.0
130.90	117.0
134.90	231.0
136.90	235.0
140.80	1097.0
141.90	114.0
142.80	1455.0
144.80	192.0
145.90	155.0
147.90	258.0
149.80	109.0
154.80	293.0
156.80	223.0
160.70	108.0
171.90	644.0
173.90	67648.0
174.90	4813.0
175.90	65560.0
176.90	4524.0

Instrument :
MSVOA_U
ClientSampleId :
BFB047

m/z	Abundance
35.90	994.0
37.00	3640.0
38.00	3346.0
39.00	1550.0
39.90	133.0
43.90	554.0
44.90	654.0
47.10	844.0
47.90	517.0
49.00	3554.0
50.00	15885.0
51.00	5215.0
51.90	189.0
54.90	169.0
56.00	1314.0
57.00	2658.0
58.00	103.0
59.90	826.0
61.00	4536.0
62.00	4727.0
63.00	3662.0
63.90	516.0
65.00	490.0
66.90	241.0
68.00	9756.0
69.00	10229.0
70.00	820.0
72.00	629.0
73.00	4593.0
74.00	16371.0
75.00	53168.0
76.00	4306.0
76.90	660.0
78.10	408.0
78.90	2925.0
79.80	909.0
80.90	3483.0
81.80	793.0
85.90	111.0
86.90	3781.0
88.00	3279.0
90.90	365.0
92.00	2878.0
92.90	4142.0
94.00	12254.0
95.00	99312.0
96.00	6488.0
96.90	287.0
103.80	437.0
104.80	140.0
105.90	412.0
106.80	127.0
110.80	116.0
114.80	130.0
115.80	319.0
116.80	899.0
117.80	456.0
118.80	638.0
127.80	334.0
128.70	175.0
129.90	382.0
130.90	134.0
134.90	214.0
136.90	225.0
140.80	1154.0
141.80	111.0
142.80	1582.0
144.80	230.0
145.90	197.0
146.80	100.0
147.90	269.0
149.80	108.0
154.80	295.0
156.80	208.0
160.80	137.0
171.90	639.0
173.90	73408.0
174.90	5186.0
175.90	70104.0
176.90	4741.0

Instrument :
MSVOA_U
ClientSampleId :
BFB047

m/z	Abundance
35.90	976.0
37.00	3542.0
38.00	3222.0
39.00	1478.0
40.00	188.0
43.90	565.0
44.90	624.0
47.00	821.0
47.90	490.0
49.00	3283.0
50.00	15042.0
51.00	4853.0
51.90	201.0
54.90	210.0
56.00	1213.0
57.00	2550.0
59.90	859.0
61.00	4259.0
62.00	4422.0
63.00	3511.0
63.90	480.0
65.00	457.0
67.00	210.0
68.00	9106.0
69.00	10020.0
70.00	844.0
72.00	580.0
73.00	4559.0
74.00	15926.0
75.00	50840.0
76.00	4182.0
76.80	623.0
78.10	303.0
78.90	2810.0
79.80	845.0
80.90	3225.0
81.80	742.0
85.90	120.0
87.00	3741.0
88.00	3229.0
90.80	343.0
91.90	2851.0
92.90	3867.0
94.00	11743.0
95.00	95944.0
96.00	6053.0
96.90	273.0
103.80	412.0
104.90	166.0
105.90	422.0
106.70	113.0
110.80	126.0
114.80	140.0
115.70	308.0
116.80	796.0
117.80	456.0
118.80	591.0
127.90	320.0
128.70	183.0
129.90	356.0
130.80	145.0
134.80	186.0
136.90	204.0
140.90	1123.0
141.90	103.0
142.80	1493.0
144.90	248.0
145.90	166.0
147.80	242.0
154.80	249.0
156.80	167.0
160.80	156.0
171.90	653.0
173.90	72560.0
174.90	5248.0
175.90	68480.0
176.90	4468.0
177.80	112.0

Instrument :
MSVOA_U
ClientSampleId :
BFB047