

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121824\
 Data File : VU062430.D
 Acq On : 18 Dec 2024 18:43
 Operator : MD/SY
 Sample : P5309-09
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CG4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU062430.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.358	15	21	29	rBV2	9572	10043	3.62%	0.406%
2	1.596	83	95	110	rVB	35148	46732	16.83%	1.889%
3	1.907	183	192	210	rVB	25742	34208	12.32%	1.383%
4	2.075	235	244	261	rBV	43819	62636	22.55%	2.531%
5	2.560	383	395	412	rVB	58880	96183	34.63%	3.887%
6	2.679	412	432	444	rVB4	8045	16888	6.08%	0.683%
7	4.563	1009	1018	1029	rBV2	4475	9778	3.52%	0.395%
8	4.631	1029	1039	1065	rVV	30736	82231	29.61%	3.323%
9	5.052	1156	1170	1195	rBV	59206	132300	47.63%	5.347%
10	5.714	1358	1376	1399	rBV2	105556	277743	100.00%	11.225%
11	6.242	1528	1540	1574	rBV	100799	199023	71.66%	8.044%
12	6.541	1623	1633	1650	rBB5	8059	15861	5.71%	0.641%
13	6.682	1664	1677	1700	rBV2	63417	125796	45.29%	5.084%
14	7.560	1940	1950	1980	rBB2	31071	58225	20.96%	2.353%
15	7.891	2041	2053	2070	rBV	129837	232893	83.85%	9.413%
16	7.965	2070	2076	2093	rVB2	5838	11162	4.02%	0.451%
17	8.177	2132	2142	2154	rBV	18968	32917	11.85%	1.330%
18	8.631	2271	2283	2311	rBV3	108229	244930	88.19%	9.899%
19	9.409	2513	2525	2551	rBV	140524	246056	88.59%	9.945%
20	10.746	2929	2941	2961	rBB2	52305	84697	30.49%	3.423%
21	11.804	3259	3270	3294	rBV	136352	225327	81.13%	9.107%
22	12.068	3343	3352	3360	rBV4	2533	4627	1.67%	0.187%
23	12.184	3377	3388	3409	rBV	126105	215807	77.70%	8.722%
24	12.884	3599	3606	3617	rBV6	4857	8203	2.95%	0.332%

Sum of corrected areas: 2474266




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121824\
Data File : VU062430.D
Acq On : 18 Dec 2024 18:43
Operator : MD/SY
Sample : P5309-09
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CG4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

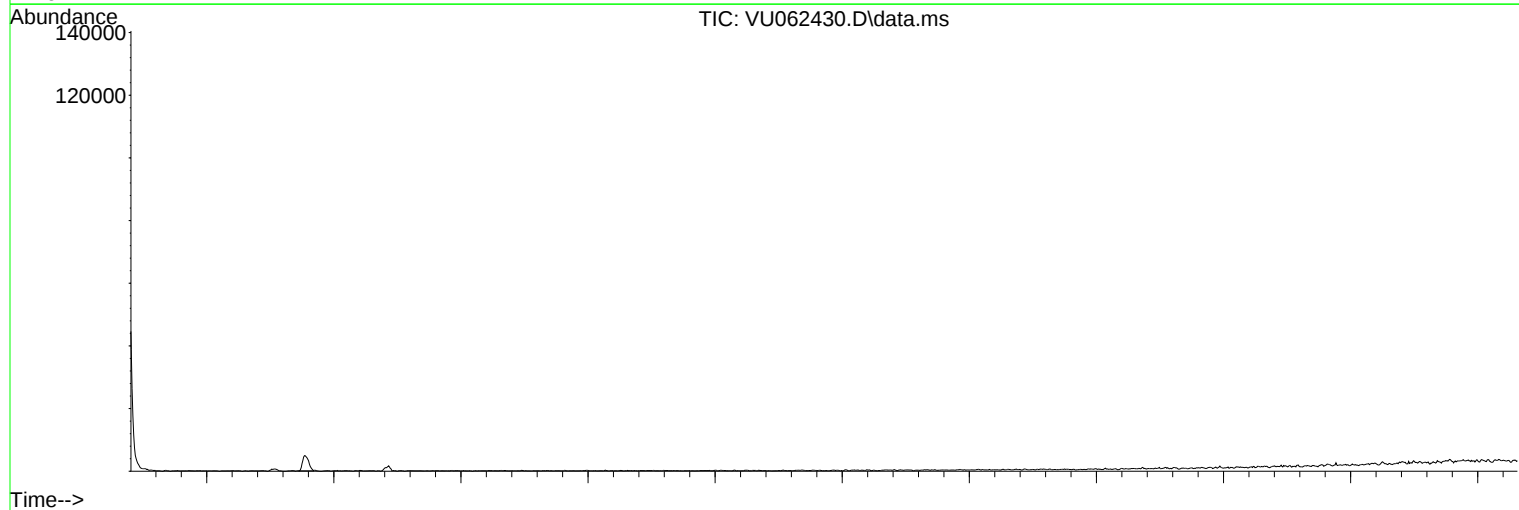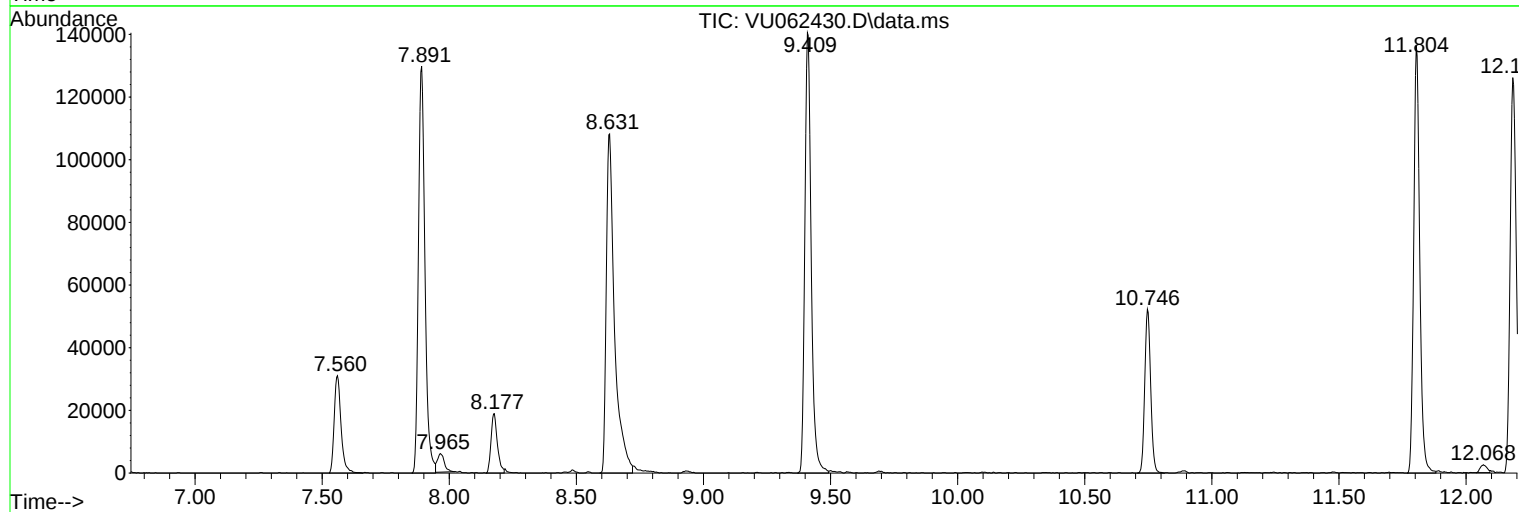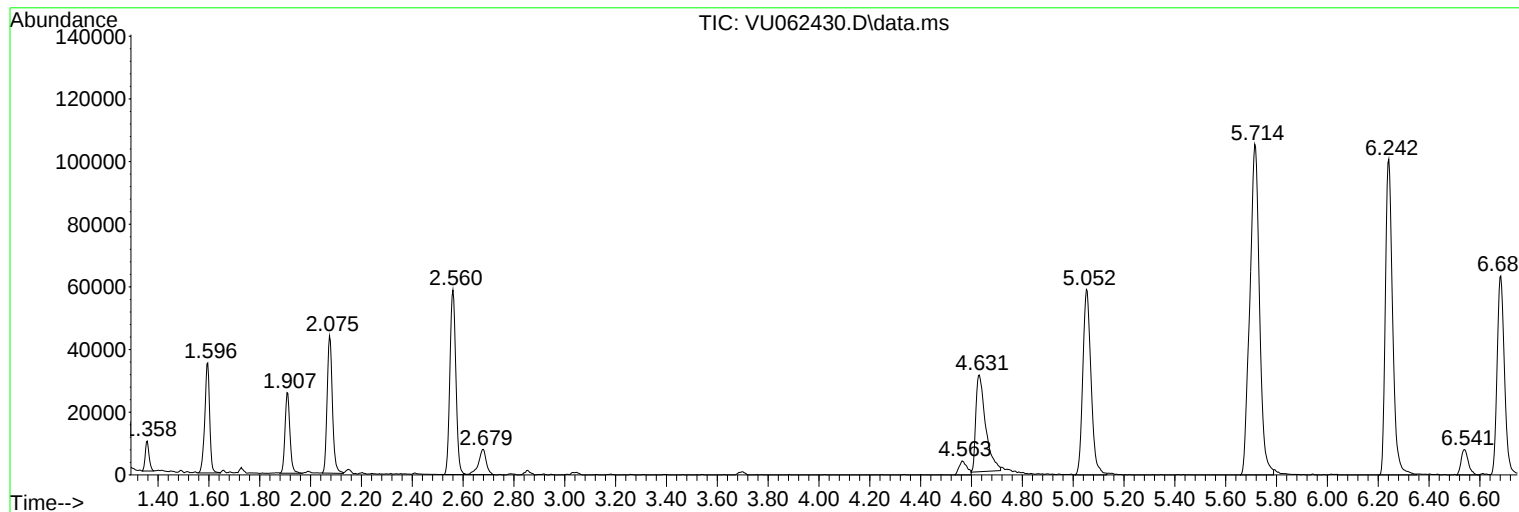

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121824\
Data File : VU062430.D
Acq On : 18 Dec 2024 18:43
Operator : MD/SY
Sample : P5309-09
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CG4










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Fluorodichloromethane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.075	1.57 ug/L	62636	1,4-Difluorobenzene	6.242

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Fluorodichloromethane	102	CHCl2F	000075-43-4	91
2	Fluorodichloromethane	102	CHCl2F	000075-43-4	91
3	Fluorodichloromethane	102	CHCl2F	000075-43-4	91
4	Cyclopentene, 1-chloro-	102	C5H7Cl	000930-29-0	5
5	Methanamine, N,N-difluoro-	67	CH3F2N	000753-58-2	5

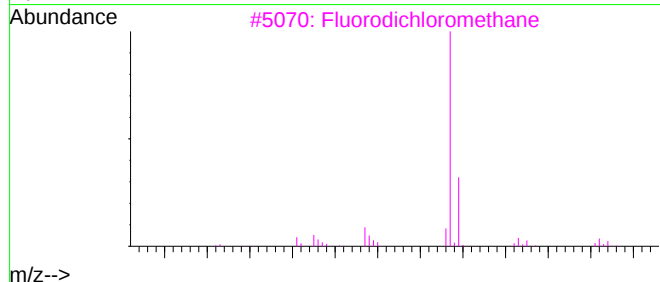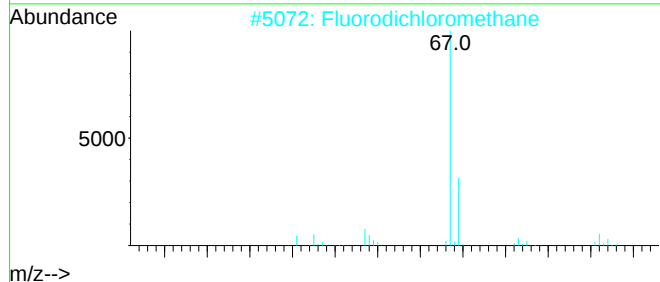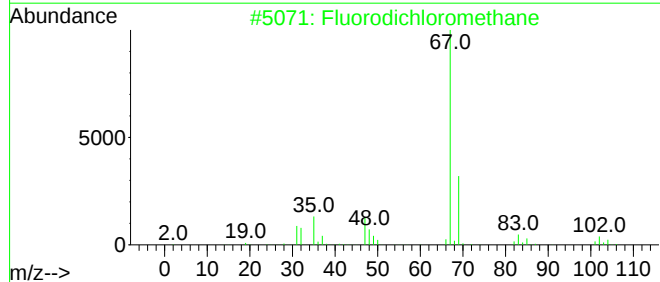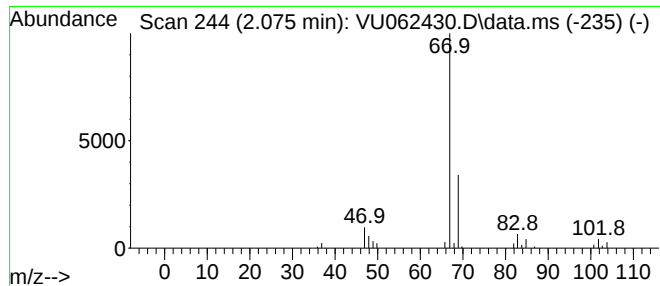

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121824\
Data File : VU062430.D
Acq On : 18 Dec 2024 18:43
Operator : MD/SY
Sample : P5309-09
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CG4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Fluorodichlorom...	2.075	1.6	ug/L	62636	1	6.242	199023	5.0