

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121824\
 Data File : VU062451.D
 Acq On : 19 Dec 2024 04:35
 Operator : MD/SY
 Sample : P5308-06
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CC6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU062451.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	86	95	111	rVB	26709	31133	12.54%	1.390%
2	1.907	183	192	206	rBV	21997	28849	11.62%	1.288%
3	2.075	235	244	253	rBV	6726	8908	3.59%	0.398%
4	2.133	253	262	272	rVB	15849	22504	9.07%	1.005%
5	2.560	382	395	413	rVB	50866	83207	33.52%	3.714%
6	4.631	1030	1039	1065	rBV	32160	90369	36.40%	4.034%
7	5.055	1156	1171	1200	rBV2	51715	121578	48.98%	5.427%
8	5.714	1358	1376	1402	rBV3	93566	248242	100.00%	11.082%
9	6.242	1528	1540	1567	rBV2	91330	178827	72.04%	7.983%
10	6.534	1620	1631	1648	rBV2	38382	74238	29.91%	3.314%
11	6.682	1665	1677	1694	rBV	57188	113374	45.67%	5.061%
12	7.560	1940	1950	1976	rBB	27983	50131	20.19%	2.238%
13	7.891	2041	2053	2076	rBV	114004	203060	81.80%	9.065%
14	8.174	2132	2141	2165	rBB2	16616	29668	11.95%	1.324%
15	8.396	2203	2210	2219	rBB3	2672	4051	1.63%	0.181%
16	8.547	2248	2257	2267	rBB4	9770	16700	6.73%	0.745%
17	8.631	2272	2283	2315	rBV3	106265	244853	98.63%	10.930%
18	9.409	2514	2525	2550	rBV	128548	222391	89.59%	9.928%
19	10.746	2930	2941	2959	rBB	48234	80175	32.30%	3.579%
20	11.804	3259	3270	3292	rBV2	121142	202095	81.41%	9.022%
21	12.187	3377	3389	3412	rBV	109757	185779	74.84%	8.293%




Sum of corrected areas: 2240132

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121824\
Data File : VU062451.D
Acq On : 19 Dec 2024 04:35
Operator : MD/SY
Sample : P5308-06
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

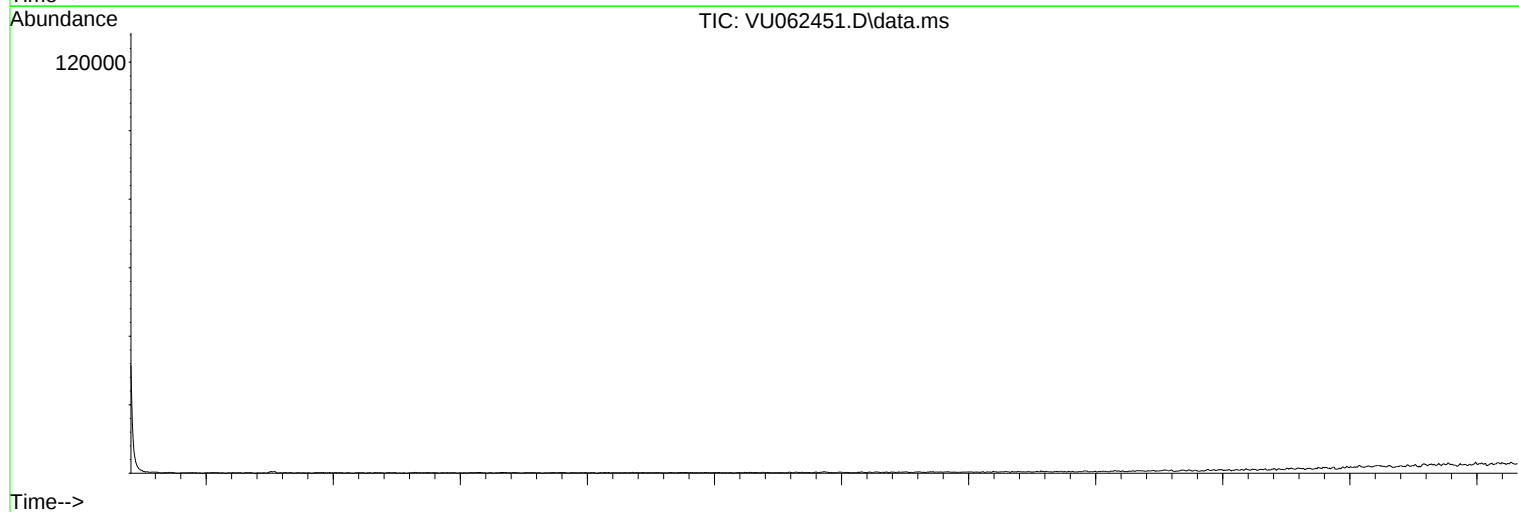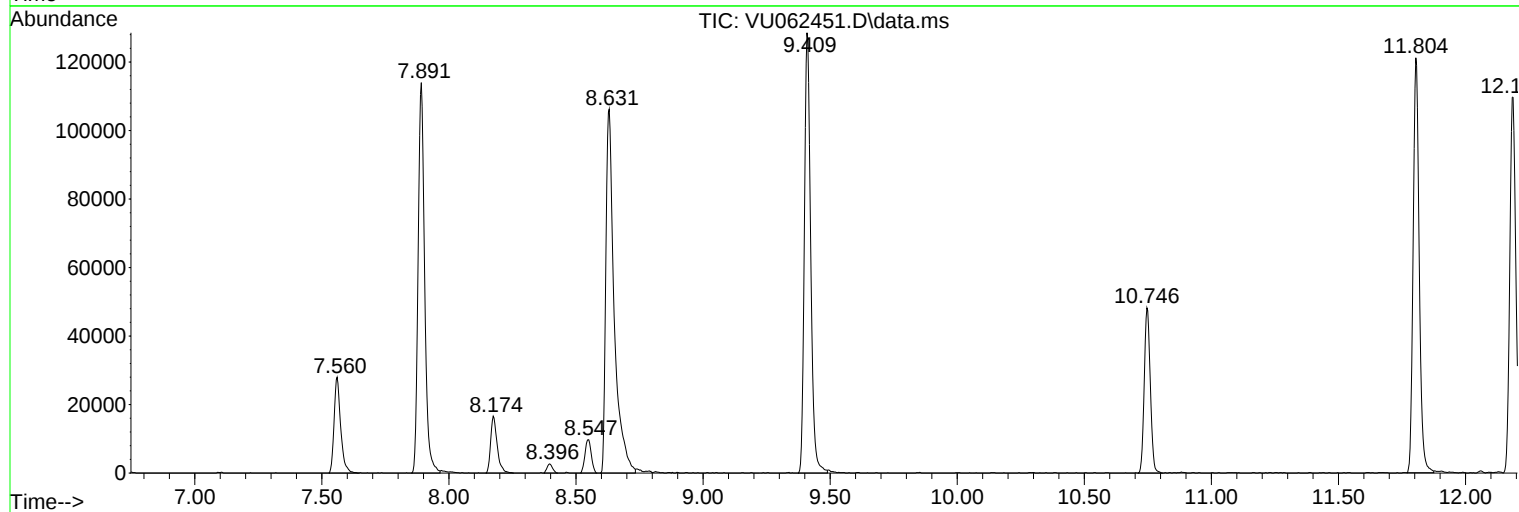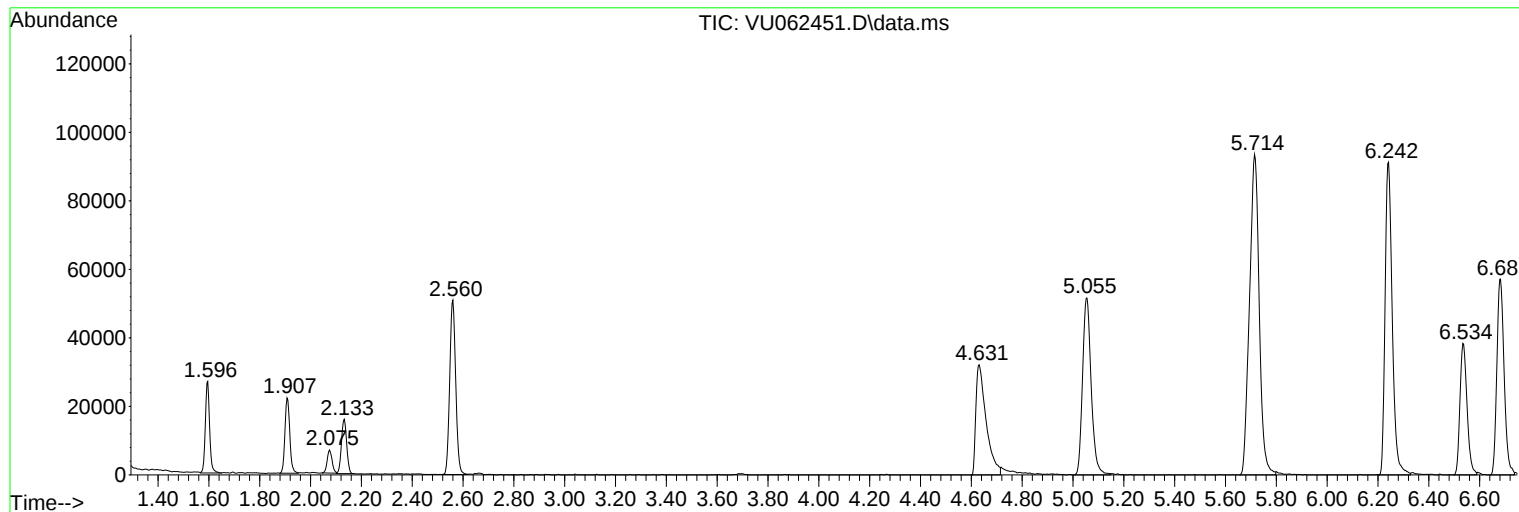

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121824\
Data File : VU062451.D
Acq On : 19 Dec 2024 04:35
Operator : MD/SY
Sample : P5308-06
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121824\
Data File : VU062451.D
Acq On : 19 Dec 2024 04:35
Operator : MD/SY
Sample : P5308-06
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------