
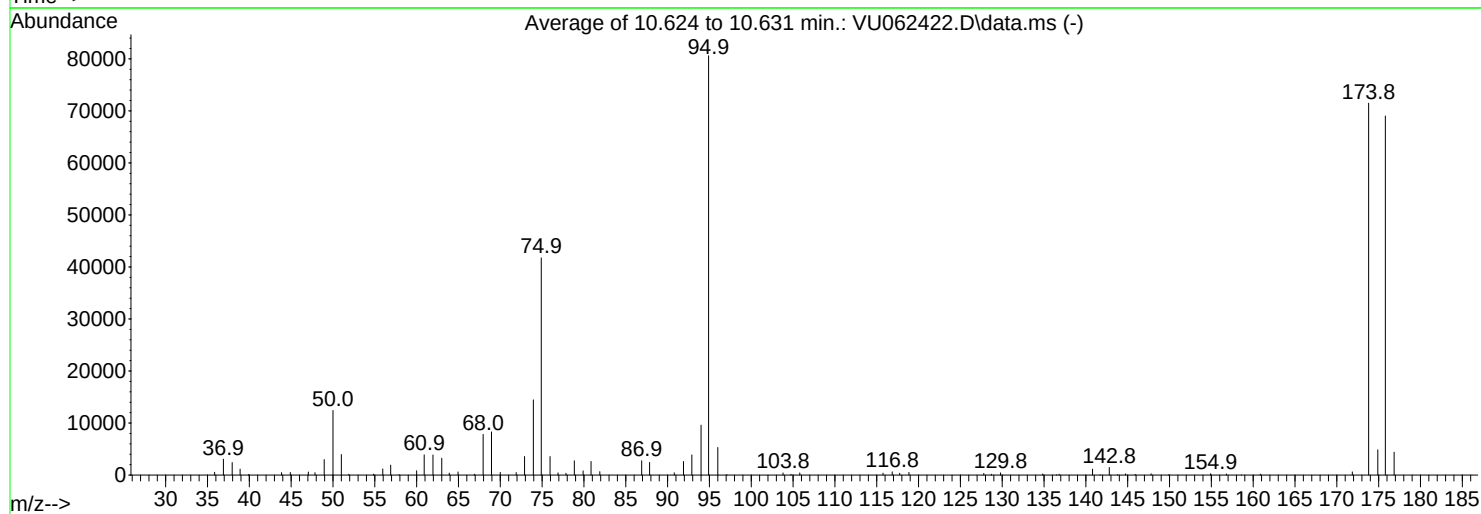


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121824\
Data File : VU062422.D
Acq On : 18 Dec 2024 14:38
Operator : MD/SY
Sample : BFB049
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB049

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Dec 20 01:26:48 2024

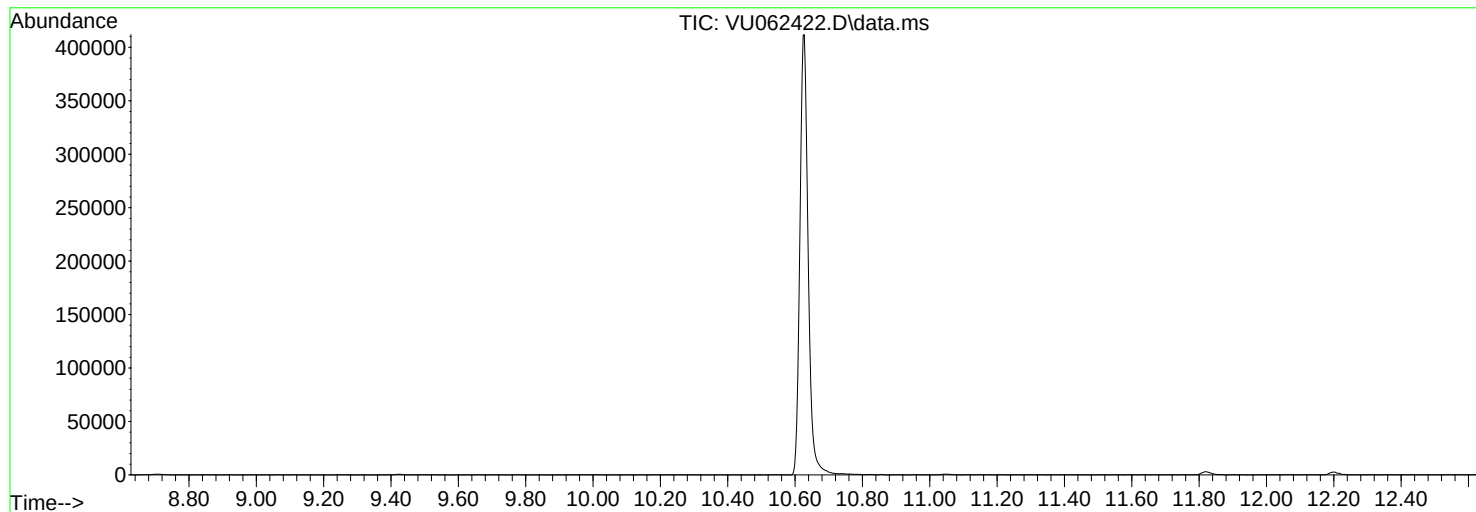

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	12423	PASS
75	95	30	80	51.8	41755	PASS
95	95	100	100	100.0	80605	PASS
96	95	5	9	6.6	5307	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.7	71485	PASS
175	174	5	9	6.8	4866	PASS
176	174	95	101	96.6	69027	PASS
177	176	5	9	6.4	4402	PASS

m/z

Abundance

Instrument :

MSVOA_U

ClientSampleId :

BFB049

m/z	Abundance
35.80	530.0
36.90	3174.0
38.00	2576.0
38.90	1132.0
43.90	509.0
44.80	481.0
47.10	654.0
47.90	534.0
49.00	3158.0
50.00	12949.0
51.00	4125.0
51.90	223.0
54.90	179.0
55.90	1239.0
56.90	2041.0
60.00	926.0
60.90	4115.0
61.90	4077.0
63.00	3490.0
63.90	460.0
65.00	685.0
66.90	191.0
67.90	8455.0
68.90	8821.0
70.00	561.0
71.90	508.0
72.90	3814.0
74.00	15100.0
74.90	43088.0
75.90	3838.0
76.90	423.0
77.80	376.0
78.90	2900.0
79.90	866.0
80.90	2781.0
81.90	727.0
86.90	2878.0
87.80	2518.0
90.80	467.0
91.90	2666.0
92.90	3987.0
94.00	10156.0
94.90	82432.0
96.00	5421.0
97.10	120.0
103.80	381.0
104.80	169.0
105.80	457.0
115.70	384.0
116.80	633.0
117.80	384.0
118.90	462.0
127.80	315.0
128.70	177.0
129.80	425.0
134.90	239.0
136.80	198.0
140.80	1101.0
141.70	131.0
142.80	1480.0
144.80	262.0
145.90	120.0
147.80	224.0
149.90	104.0
154.90	195.0
156.80	235.0
160.90	175.0
171.90	656.0
173.80	72680.0
174.90	5112.0
175.80	69880.0
176.90	4342.0

Instrument :
MSVOA_U
ClientSampleId :
BFB049

m/z	Abundance
35.90	545.0
36.90	3162.0
38.00	2433.0
38.90	1176.0
39.90	120.0
43.80	492.0
44.90	516.0
47.10	602.0
47.90	483.0
48.90	3109.0
50.00	12632.0
51.00	4100.0
51.90	165.0
54.80	179.0
55.90	1245.0
56.90	1995.0
57.90	107.0
60.00	881.0
60.90	3967.0
61.90	3969.0
63.00	3406.0
63.90	381.0
65.00	635.0
66.90	189.0
68.00	8088.0
69.00	8485.0
70.00	532.0
71.90	508.0
72.90	3627.0
73.90	14808.0
74.90	42944.0
75.90	3667.0
76.90	429.0
77.80	388.0
78.80	2817.0
79.90	840.0
80.90	2713.0
81.90	704.0
86.90	2858.0
87.80	2521.0
90.80	470.0
91.90	2666.0
92.90	3984.0
94.00	9879.0
94.90	83216.0
96.00	5439.0
97.10	105.0
103.80	435.0
104.80	153.0
105.80	422.0
115.80	392.0
116.80	650.0
117.80	367.0
118.90	523.0
127.80	336.0
128.70	161.0
129.80	466.0
134.80	228.0
136.80	165.0
140.80	1167.0
142.80	1535.0
143.80	113.0
144.70	270.0
145.90	131.0
147.80	284.0
149.90	103.0
154.90	280.0
156.80	225.0
158.60	106.0
160.80	197.0
171.90	619.0
173.80	73800.0
174.90	4939.0
175.80	71096.0
176.90	4537.0

Instrument :
MSVOA_U
ClientSampleId :
BFB049

m/z	Abundance
35.90	557.0
36.90	2822.0
37.90	2226.0
38.90	1152.0
39.90	152.0
43.90	417.0
45.00	508.0
46.90	517.0
47.70	406.0
48.90	2680.0
50.00	11688.0
51.00	3621.0
52.00	115.0
54.80	176.0
56.00	1097.0
56.90	1698.0
57.90	116.0
60.00	708.0
60.90	3597.0
62.00	3553.0
63.00	2826.0
63.90	323.0
64.90	525.0
66.90	166.0
67.90	6947.0
69.00	7583.0
70.00	495.0
71.90	448.0
72.90	3263.0
73.90	13482.0
74.90	39232.0
76.00	3216.0
76.90	447.0
77.90	330.0
78.90	2545.0
79.90	733.0
80.80	2381.0
81.90	582.0
86.90	2538.0
87.90	2258.0
90.80	391.0
91.90	2495.0
92.90	3668.0
94.00	8755.0
94.90	76168.0
96.00	5060.0
103.80	434.0
104.70	127.0
105.80	360.0
115.80	357.0
116.90	622.0
117.70	318.0
118.80	570.0
127.80	311.0
128.70	154.0
129.80	427.0
134.80	212.0
136.50	142.0
136.80	124.0
140.80	1127.0
142.80	1389.0
143.80	133.0
144.70	211.0
145.90	159.0
147.80	264.0
154.90	307.0
156.80	185.0
160.80	189.0
171.80	582.0
173.80	67976.0
174.90	4547.0
175.80	66104.0
176.80	4327.0

Instrument :
MSVOA_U
ClientSampleId :
BFB049