

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121924\
 Data File : VU062473.D
 Acq On : 19 Dec 2024 14:19
 Operator : MD/SY
 Sample : P5309-08
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CG3

Quant Time: Dec 20 00:38:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Dec 20 00:36:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	83814	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	79986	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	38008	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	24380	4.312	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.200%
7) Chloroethane-d5	1.908	69	19024	4.731	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.600%
11) 1,1-Dichloroethene-d2	2.560	65	12741	4.737	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	94.800%
20) 2-Butanone-d5	4.624	46	43791	40.418	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	80.840%
24) Chloroform-d	5.052	84	57654	4.712	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.200%
26) 1,2-Dichloroethane-d4	5.692	65	31083	5.166	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.400%
32) Benzene-d6	5.718	84	102646	4.456	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.200%
36) 1,2-Dichloropropane-d6	6.679	67	28051	4.256	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.200%
41) Toluene-d8	7.891	98	95472	4.387	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.800%
43) trans-1,3-Dichloroprop...	8.174	79	12967	4.469	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.400%
46) 2-Hexanone-d5	8.628	63	32397	37.012	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	74.020%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	21757	4.242	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.800%
66) 1,2-Dichlorobenzene-d4	12.184	152	35018	5.000	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.000%
Target Compounds					Qvalue	
13) Acetone	2.650	43	3130	4.243	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121924\
Data File : VU062473.D
Acq On : 19 Dec 2024 14:19
Operator : MD/SY
Sample : P5309-08
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CG3


Quant Time: Dec 20 00:38:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Dec 20 00:36:00 2024
Response via : Initial Calibration

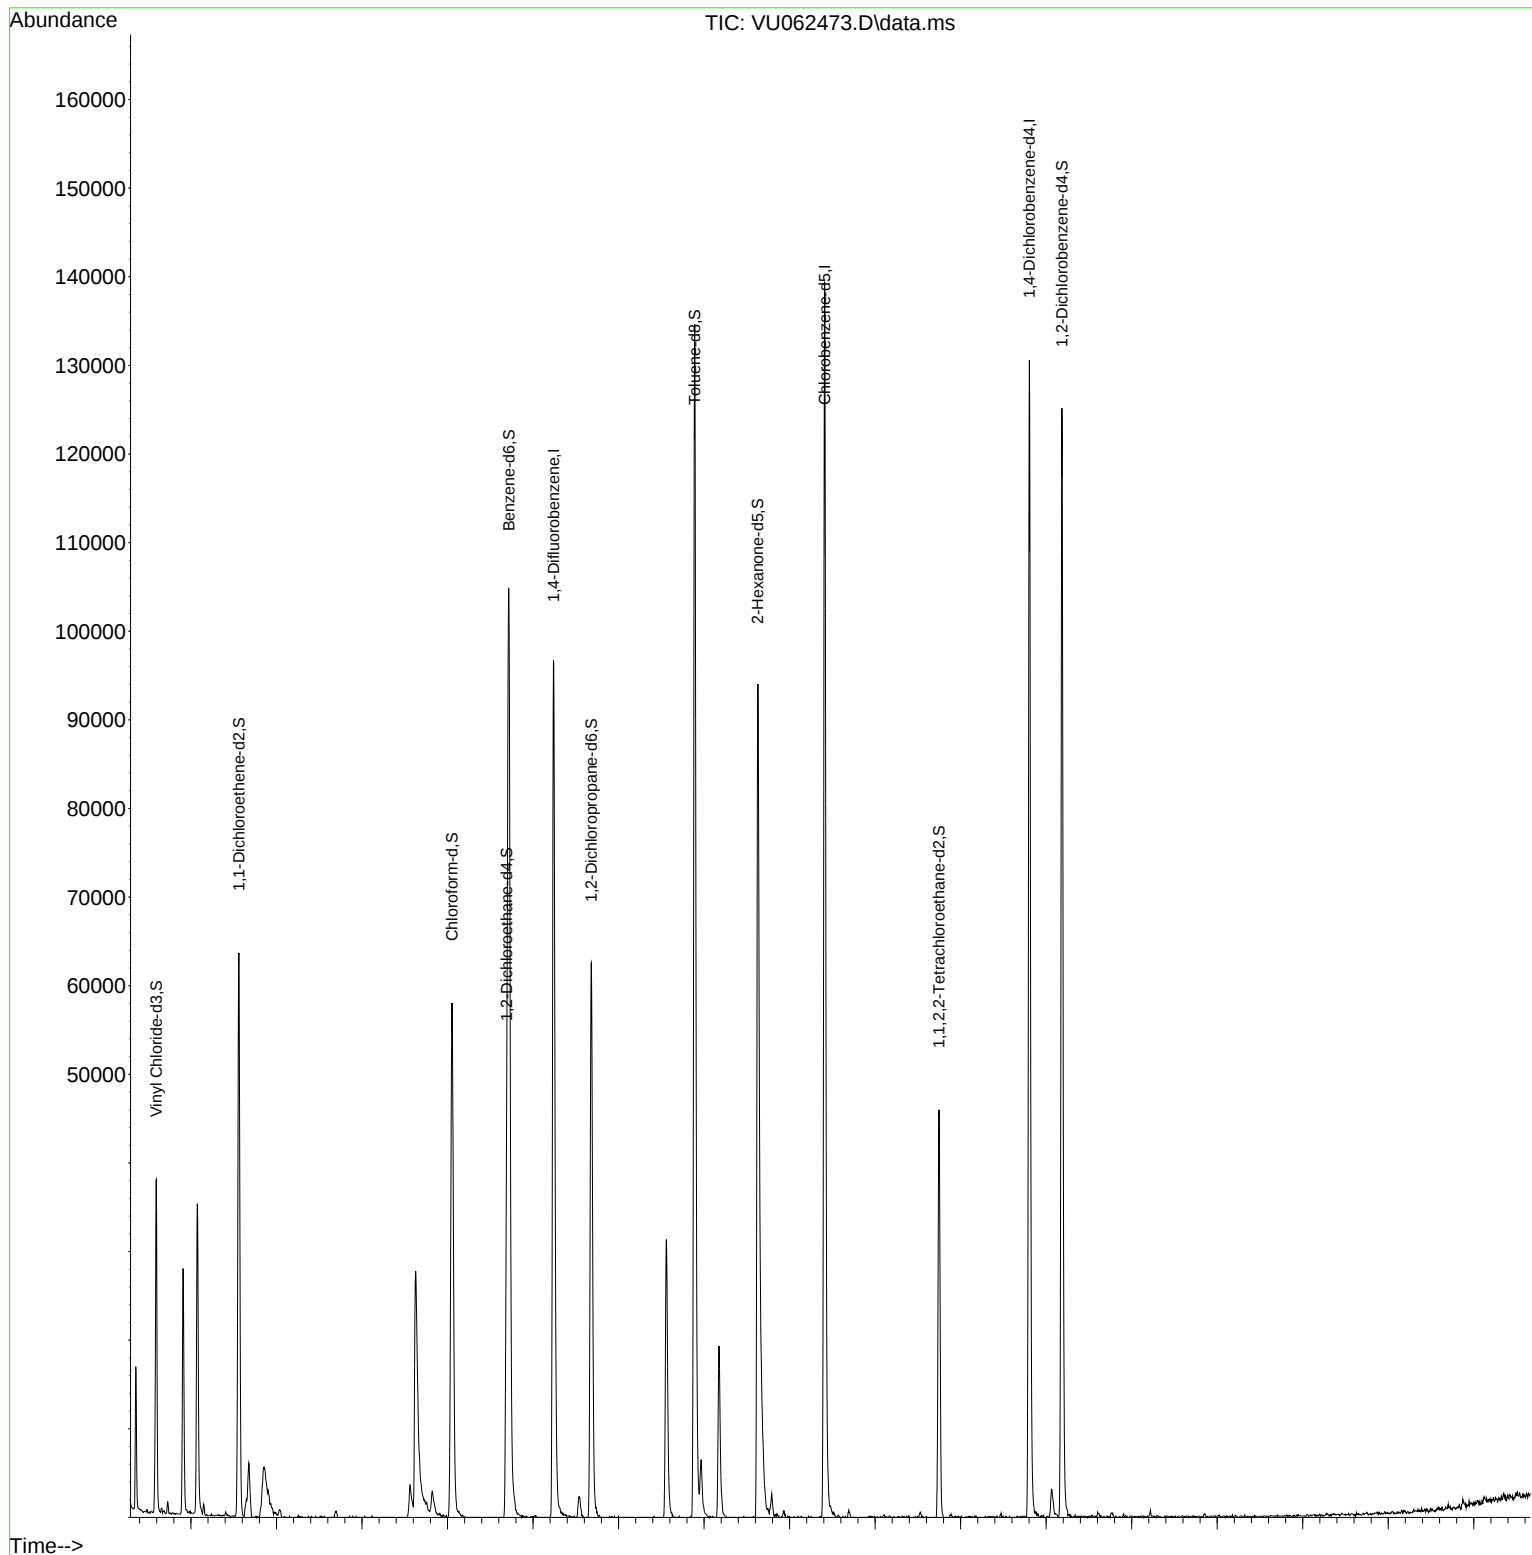

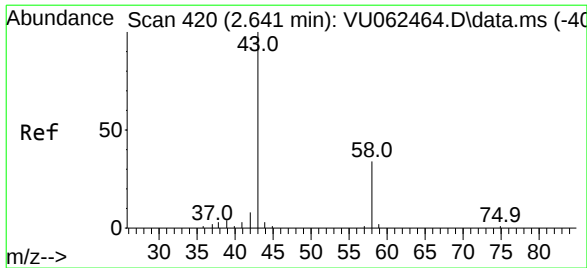

#13
 Acetone
 Concen: 4.243 ug/L
 RT: 2.650 min Scan# 42
 Delta R.T. 0.010 min
 Lab File: VU062473.D
 Acq: 19 Dec 2024 14:19

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CG3

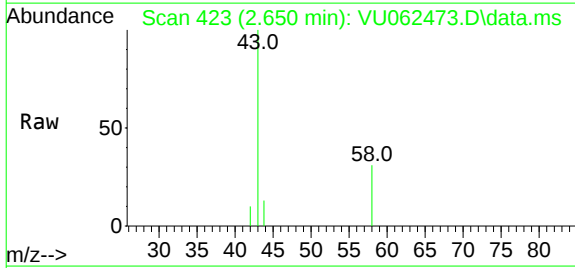

Tgt Ion: 43 Resp: 3130
 Ion Ratio Lower Upper
 43 100
 58 27.8 0.0 64.0

