

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121924\
 Data File : VU062492.D
 Acq On : 20 Dec 2024 01:05
 Operator : MD/SY
 Sample : P5308-10
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CD1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU062492.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	85	95	104	rBV	34988	41616	1.17%	0.667%
2	2.075	235	244	254	rBV	31466	44401	1.24%	0.712%
3	2.560	383	395	415	rBB	60276	99824	2.80%	1.601%
4	4.653	1030	1046	1081	rBV2	168050	439457	12.32%	7.047%
5	5.052	1156	1170	1196	rBV	54042	123436	3.46%	1.979%
6	5.714	1358	1376	1397	rBV3	99346	260237	7.29%	4.173%
7	6.238	1528	1539	1565	rBV	98919	190931	5.35%	3.062%
8	6.531	1616	1630	1666	rBV	1882480	3568349	100.00%	57.219%
9	6.679	1666	1676	1701	rVB2	60179	121747	3.41%	1.952%
10	7.560	1939	1950	1970	rBV2	28501	53608	1.50%	0.860%
11	7.891	2041	2053	2073	rBV	128061	228403	6.40%	3.662%
12	8.544	2245	2256	2273	rBV2	86368	148974	4.17%	2.389%
13	8.627	2273	2282	2312	rBV2	86458	198081	5.55%	3.176%
14	9.409	2514	2525	2542	rBV	138447	239740	6.72%	3.844%
15	10.746	2931	2941	2956	rBV	43914	71127	1.99%	1.141%
16	11.804	3259	3270	3290	rBV	130480	216381	6.06%	3.470%
17	12.184	3377	3388	3407	rBV	111457	189997	5.32%	3.047%




Sum of corrected areas: 6236309

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121924\
Data File : VU062492.D
Acq On : 20 Dec 2024 01:05
Operator : MD/SY
Sample : P5308-10
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

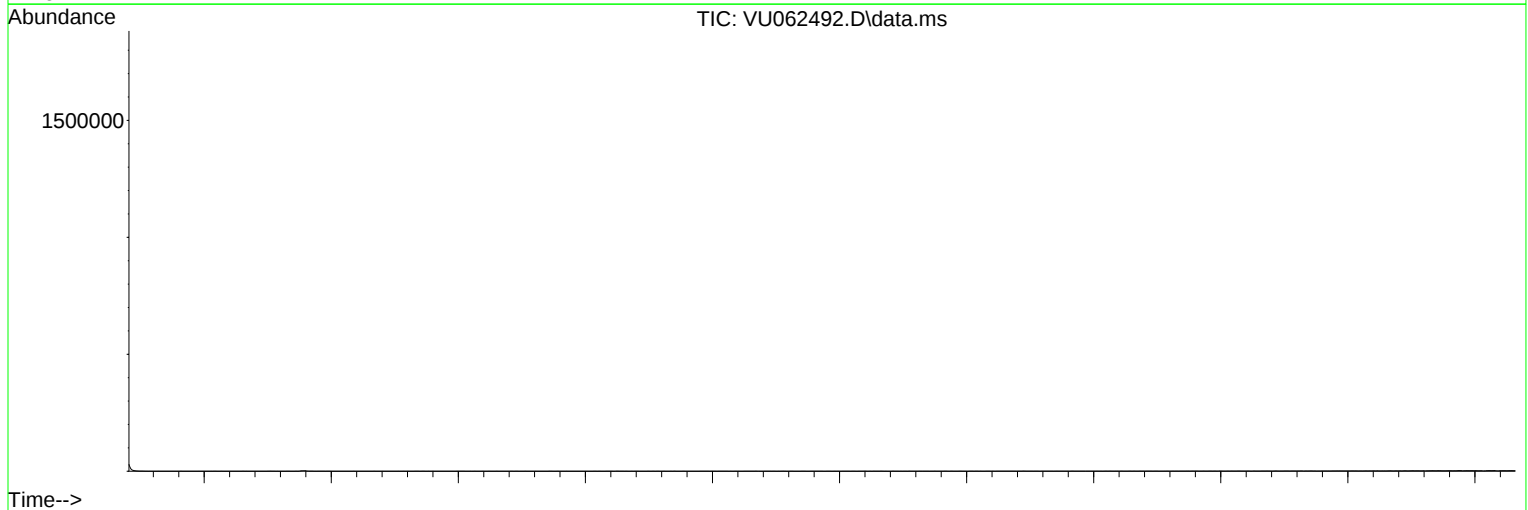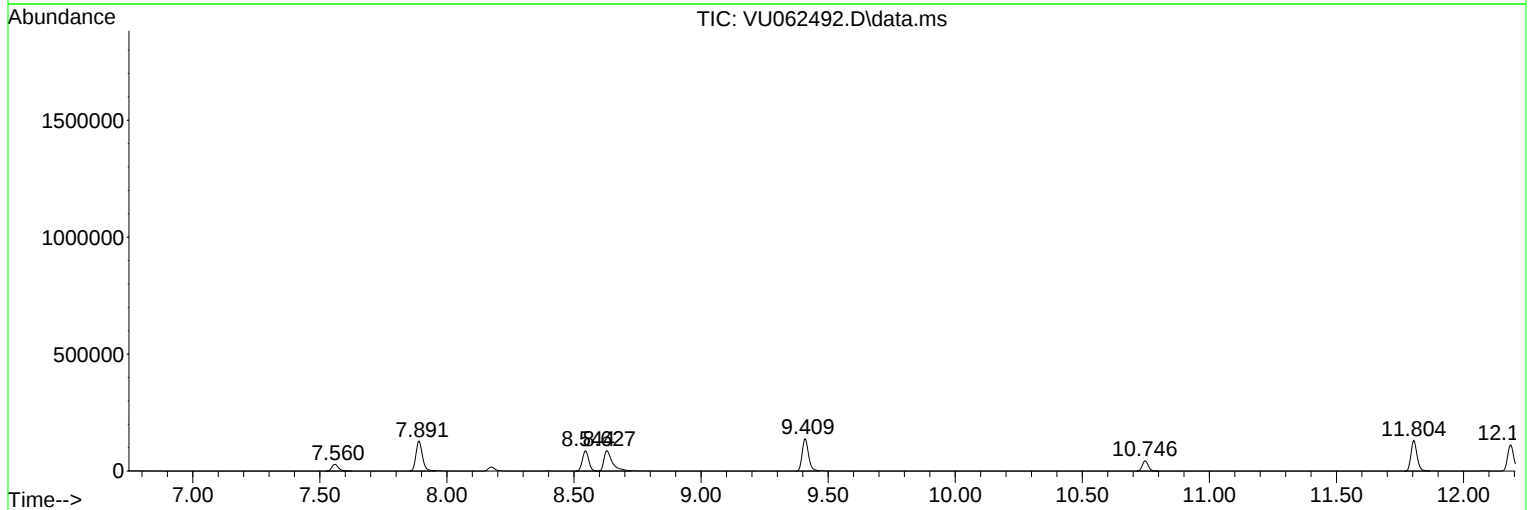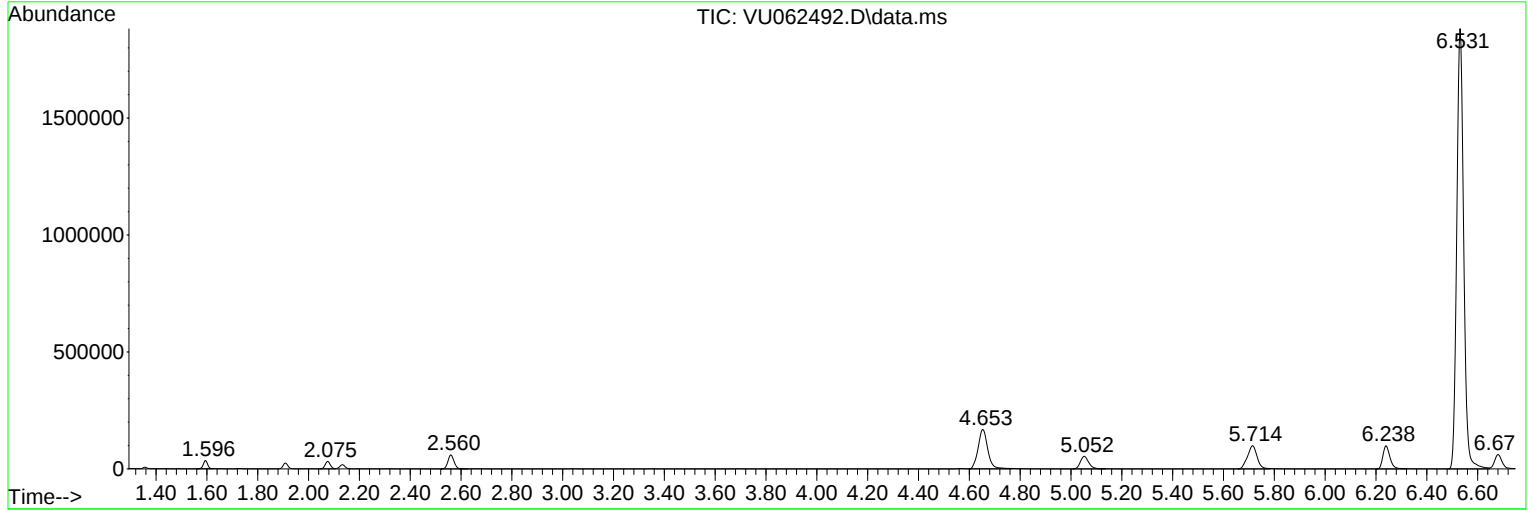

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121924\
Data File : VU062492.D
Acq On : 20 Dec 2024 01:05
Operator : MD/SY
Sample : P5308-10
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0










TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

Peak Number 1 Fluorodichloromethane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.075	1.16 ug/L	44401	1,4-Difluorobenzene	6.238

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Fluorodichloromethane	102	CHCl2F	000075-43-4	91
2	Fluorodichloromethane	102	CHCl2F	000075-43-4	91
3	Fluorodichloromethane	102	CHCl2F	000075-43-4	47
4	1-Butyne, 3,3-dimethyl-	82	C6H10	000917-92-0	7
5	Chlorine dioxide	67	ClO2	010049-04-4	5

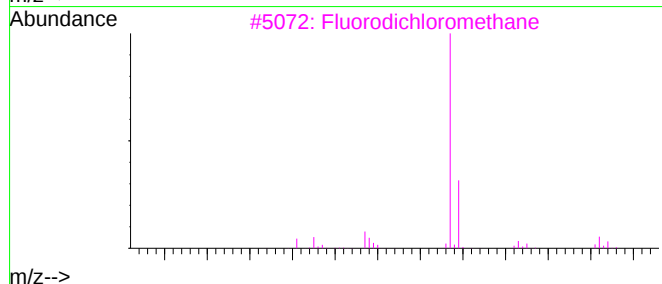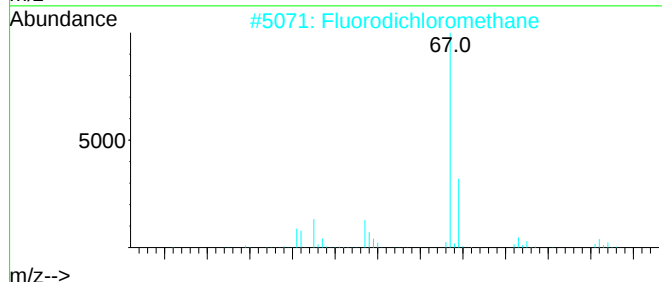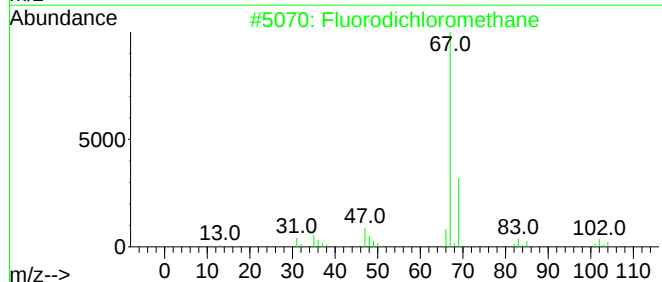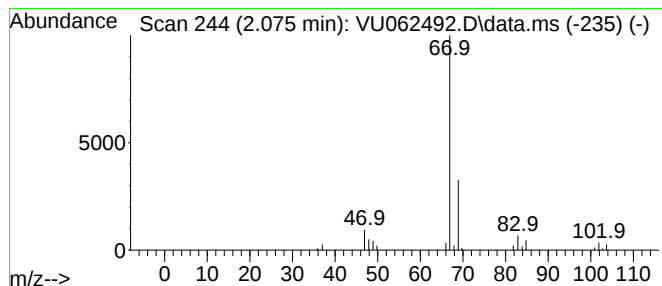

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121924\
Data File : VU062492.D
Acq On : 20 Dec 2024 01:05
Operator : MD/SY
Sample : P5308-10
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Fluorodichlorom...	2.075	1.2	ug/L	44401	1	6.238	190931	5.0