

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121924\
 Data File : VU062496.D
 Acq On : 20 Dec 2024 02:43
 Operator : MD/SY
 Sample : P5308-15
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CD6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU062496.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	83	94	109	rVB	32255	37607	15.35%	1.824%
2	1.907	180	192	204	rBV	23977	30819	12.58%	1.495%
3	2.071	234	243	260	rBV	13067	18502	7.55%	0.897%
4	2.557	383	394	412	rBV	55450	91611	37.38%	4.443%
5	2.679	419	432	442	rVB3	5477	10107	4.12%	0.490%
6	4.624	1024	1037	1069	rBV	23052	65387	26.68%	3.171%
7	5.049	1156	1169	1194	rBV2	50222	113267	46.22%	5.493%
8	5.714	1358	1376	1398	rBV2	92559	245055	100.00%	11.885%
9	6.238	1528	1539	1565	rBV	94795	183794	75.00%	8.914%
10	6.541	1626	1633	1642	rBB3	1721	2679	1.09%	0.130%
11	6.679	1665	1676	1696	rBV2	55867	109579	44.72%	5.314%
12	7.557	1940	1949	1969	rBV2	27266	49776	20.31%	2.414%
13	7.888	2041	2052	2072	rBV	118371	209959	85.68%	10.183%
14	8.171	2132	2140	2157	rBV3	15747	27998	11.43%	1.358%
15	8.631	2273	2283	2319	rBV4	78259	184227	75.18%	8.935%
16	9.409	2514	2525	2548	rBV	129154	227948	93.02%	11.055%
17	10.746	2931	2941	2958	rBV2	41610	67771	27.66%	3.287%
18	11.804	3259	3270	3293	rBV	125920	207862	84.82%	10.081%
19	12.183	3377	3388	3410	rBV	103923	177971	72.62%	8.631%

Sum of corrected areas: 2061919




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121924\
Data File : VU062496.D
Acq On : 20 Dec 2024 02:43
Operator : MD/SY
Sample : P5308-15
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

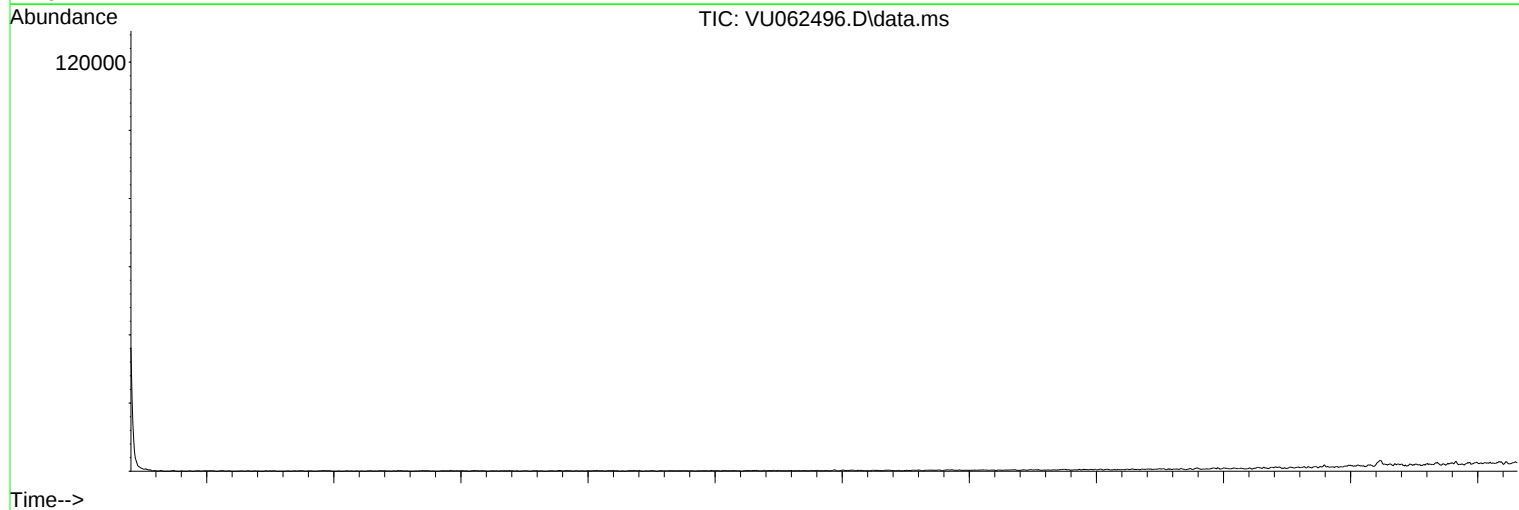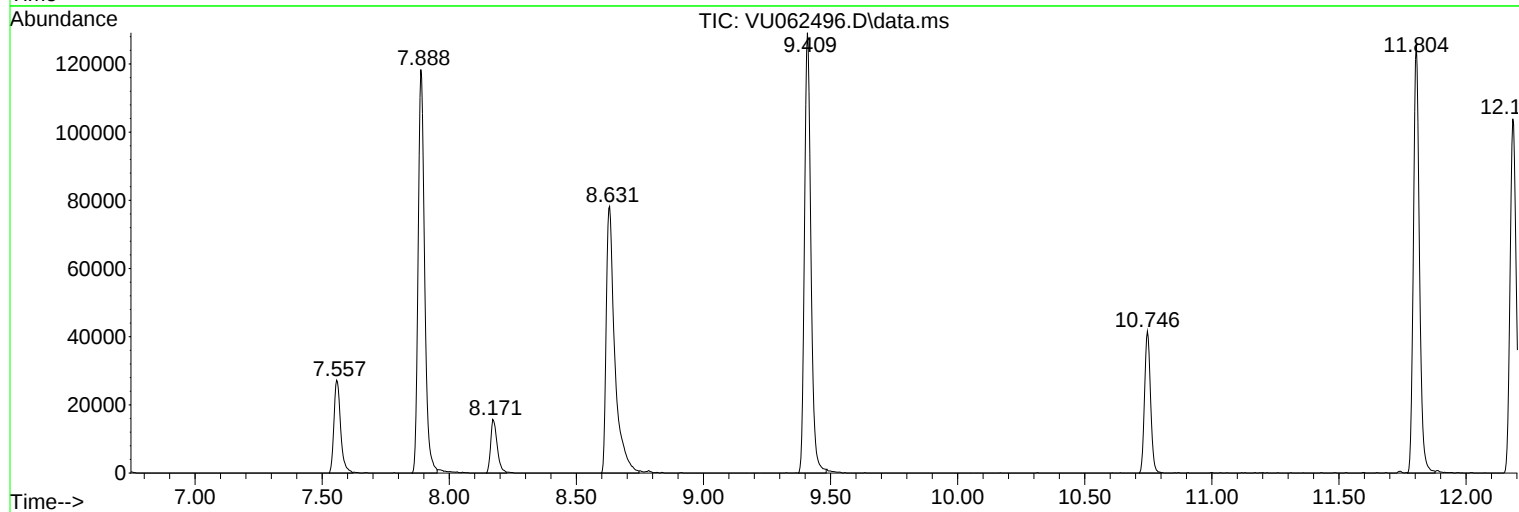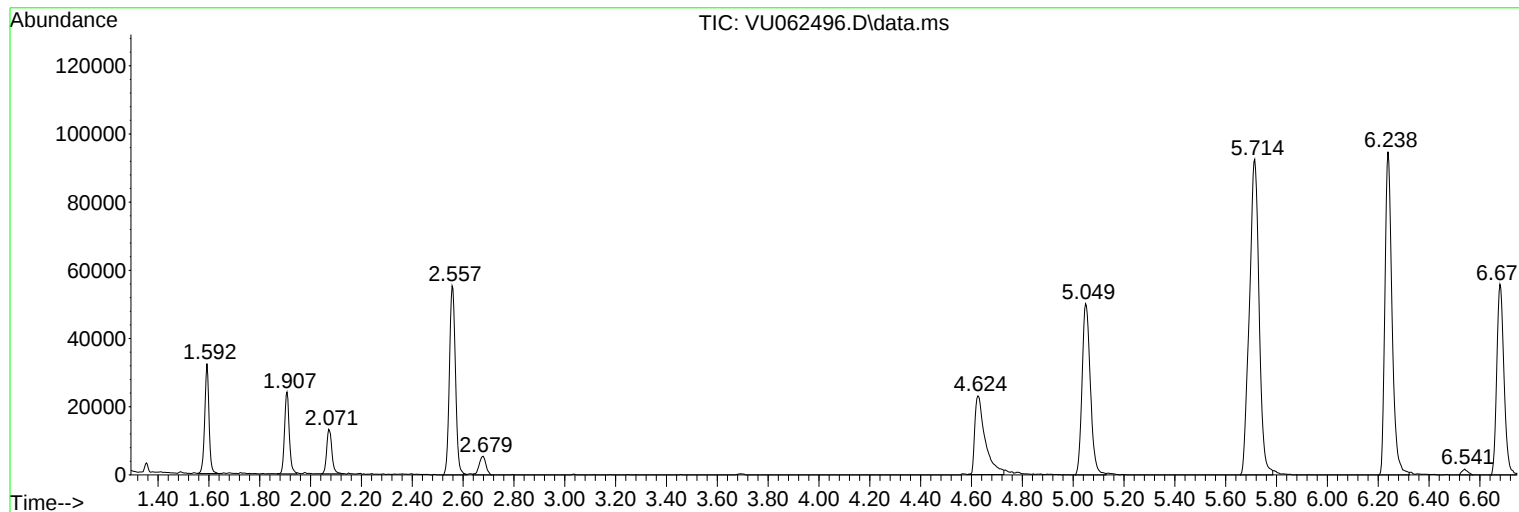

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121924\
Data File : VU062496.D
Acq On : 20 Dec 2024 02:43
Operator : MD/SY
Sample : P5308-15
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CD6










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Fluorodichloromethane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.071	0.50 ug/L	18502	1,4-Difluorobenzene	6.238

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Fluorodichloromethane	102	CHCl2F	000075-43-4	91
2	Fluorodichloromethane	102	CHCl2F	000075-43-4	91
3	Fluorodichloromethane	102	CHCl2F	000075-43-4	86
4	Cyclopentene, 1-chloro-	102	C5H7Cl	000930-29-0	5
5	Chlorine dioxide	67	ClO2	010049-04-4	5

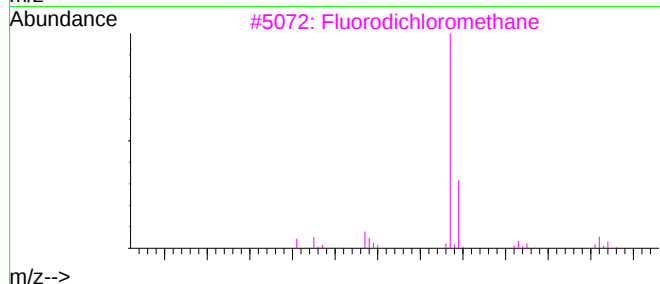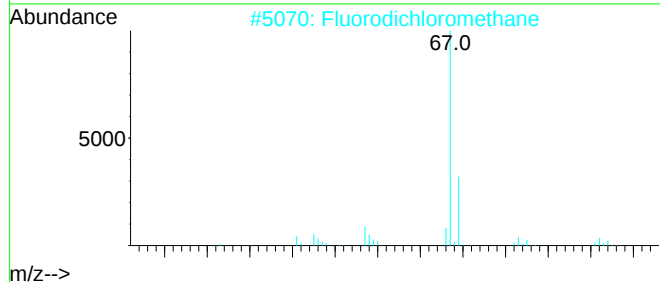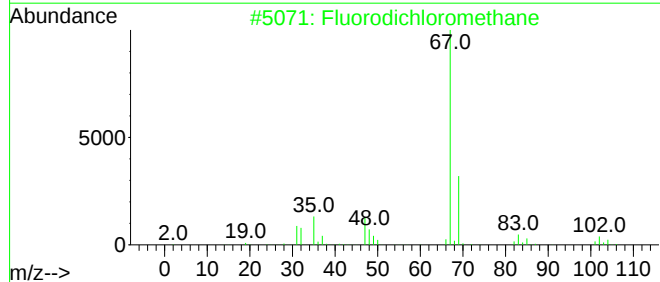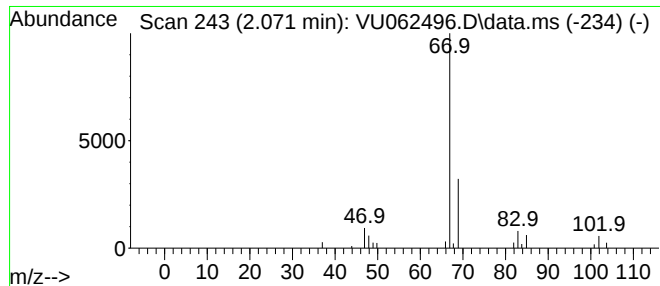

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121924\
Data File : VU062496.D
Acq On : 20 Dec 2024 02:43
Operator : MD/SY
Sample : P5308-15
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Fluorodichlorom...	2.071	0.5	ug/L	18502	1	6.238	183794	5.0