
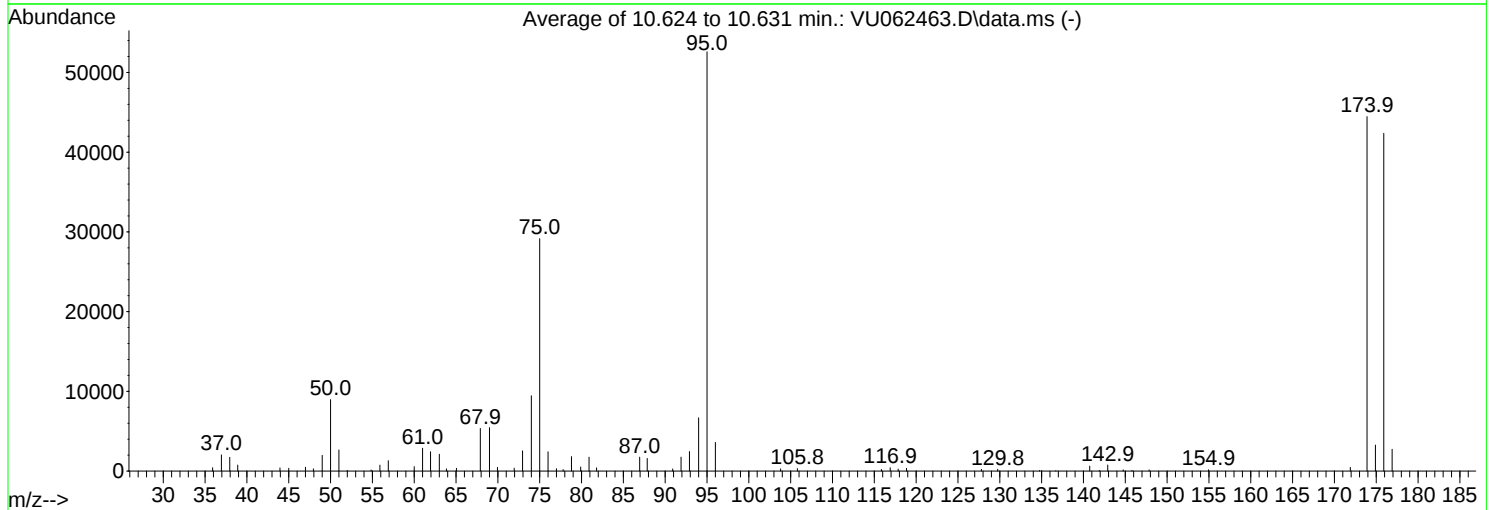


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121924\
Data File : VU062463.D
Acq On : 19 Dec 2024 09:35
Operator : MD/SY
Sample : BFB050
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB050

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Dec 20 01:26:48 2024

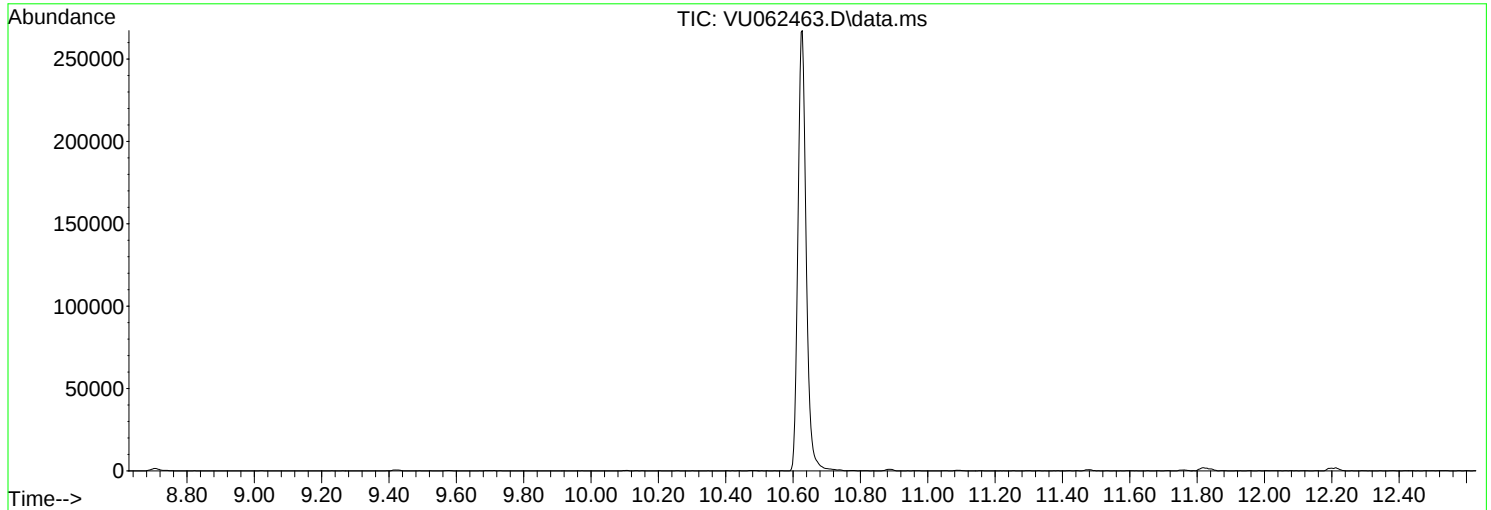

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	8969	PASS
75	95	30	80	55.4	29157	PASS
95	95	100	100	100.0	52600	PASS
96	95	5	9	6.8	3600	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.5	44467	PASS
175	174	5	9	7.3	3264	PASS
176	174	95	101	95.3	42365	PASS
177	176	5	9	6.4	2732	PASS

m/z

Abundance

Instrument :

MSVOA_U

ClientSampleId :

BFB050

m/z	Abundance
35.90	450.0
37.00	2180.0
38.00	1764.0
38.90	777.0
43.90	395.0
45.00	379.0
47.00	530.0
48.00	291.0
49.00	2048.0
50.00	9397.0
51.00	2837.0
52.00	130.0
54.80	151.0
55.90	704.0
56.90	1331.0
60.00	659.0
61.00	2897.0
61.90	2499.0
63.00	2152.0
63.80	291.0
65.00	369.0
67.90	5380.0
69.00	5932.0
70.00	507.0
72.00	308.0
73.00	2590.0
74.00	9969.0
75.00	29960.0
76.00	2725.0
77.00	353.0
77.80	203.0
78.80	1931.0
80.00	571.0
80.90	1774.0
81.80	442.0
87.00	1697.0
87.90	1755.0
90.90	259.0
91.90	1734.0
92.90	2516.0
94.00	6846.0
95.00	54040.0
96.00	3793.0
103.80	290.0
105.80	331.0
115.90	210.0
116.90	469.0
117.90	277.0
118.90	339.0
127.70	237.0
129.80	211.0
134.70	116.0
136.70	119.0
140.70	596.0
142.90	804.0
144.70	158.0
145.80	124.0
147.80	157.0
155.00	170.0
171.90	479.0
173.90	45072.0
174.90	3324.0
175.90	42600.0
176.90	2736.0

Instrument :
MSVOA_U
ClientSampleId :
BFB050

m/z	Abundance
35.90	445.0
36.90	2094.0
38.00	1762.0
38.90	776.0
44.00	413.0
45.00	351.0
47.00	516.0
48.00	287.0
49.00	2042.0
50.00	9301.0
51.00	2710.0
52.00	103.0
54.80	151.0
55.90	771.0
56.90	1337.0
60.00	573.0
61.00	3002.0
62.00	2473.0
63.00	2174.0
63.80	300.0
65.10	336.0
67.90	5520.0
69.00	5558.0
70.00	486.0
71.90	391.0
73.00	2663.0
74.00	9709.0
75.00	30032.0
76.00	2459.0
77.00	315.0
77.80	202.0
78.80	1860.0
79.90	524.0
80.90	1796.0
81.80	415.0
86.90	1802.0
87.90	1652.0
90.90	283.0
91.90	1828.0
92.90	2496.0
94.00	6836.0
95.00	54200.0
96.00	3725.0
103.80	294.0
105.80	323.0
115.80	203.0
116.90	434.0
117.80	257.0
118.80	360.0
127.80	216.0
129.70	226.0
134.80	109.0
140.80	610.0
141.90	112.0
142.90	769.0
144.80	172.0
145.80	123.0
147.90	169.0
154.90	167.0
171.90	481.0
173.90	45848.0
174.90	3393.0
175.90	43536.0
176.90	2774.0

Instrument :
MSVOA_U
ClientSampleId :
BFB050

m/z	Abundance
35.90	364.0
36.90	1843.0
37.90	1639.0
38.90	698.0
44.00	386.0
45.00	326.0
47.00	400.0
47.80	284.0
49.00	1847.0
50.00	8210.0
51.00	2397.0
54.90	109.0
55.90	764.0
56.90	1233.0
60.00	458.0
61.00	2708.0
62.00	2309.0
63.00	2024.0
63.90	270.0
65.10	325.0
67.90	5144.0
69.00	4867.0
69.90	396.0
71.90	396.0
72.90	2382.0
74.00	8664.0
75.00	27480.0
76.00	2085.0
77.00	235.0
77.80	175.0
78.80	1663.0
79.80	447.0
80.90	1675.0
81.80	357.0
86.90	1744.0
87.80	1371.0
90.90	279.0
91.90	1700.0
92.90	2341.0
94.00	6369.0
95.00	49560.0
96.00	3281.0
103.80	243.0
105.80	289.0
115.90	204.0
116.90	371.0
117.80	206.0
118.80	335.0
127.90	204.0
129.80	242.0
135.00	105.0
140.80	673.0
141.90	111.0
142.90	700.0
144.80	154.0
147.90	148.0
154.90	152.0
171.90	429.0
173.90	42480.0
174.90	3075.0
175.90	40960.0
176.90	2685.0

Instrument :
MSVOA_U
ClientSampleId :
BFB050