

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122024\
 Data File : VU062542.D
 Acq On : 21 Dec 2024 00:04
 Operator : MD/SY
 Sample : P5353-03
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E2928

Quant Time: Dec 21 01:39:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Dec 20 23:41:56 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.241	114	91638	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	89763	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	40940	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	22649	3.664	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.200%
7) Chloroethane-d5	1.907	69	18437	4.194	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.800%
11) 1,1-Dichloroethene-d2	2.560	65	12309	4.186	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	83.800%
20) 2-Butanone-d5	4.627	46	46941	39.626	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	79.260%
24) Chloroform-d	5.052	84	61868	4.625	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.400%
26) 1,2-Dichloroethane-d4	5.692	65	34128	5.188	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.800%
32) Benzene-d6	5.717	84	105647	4.086	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.800%
36) 1,2-Dichloropropane-d6	6.679	67	28854	3.901	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	78.000%
41) Toluene-d8	7.888	98	97386	3.988	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.800%
43) trans-1,3-Dichloroprop...	8.174	79	13431	4.125	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.400%
46) 2-Hexanone-d5	8.627	63	33393	33.995	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	67.980%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	22896	3.978	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	79.600%
66) 1,2-Dichlorobenzene-d4	12.183	152	36274	4.808	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.200%
Target Compounds					Qvalue	
13) Acetone	2.647	43	11510	14.271	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122024\
Data File : VU062542.D
Acq On : 21 Dec 2024 00:04
Operator : MD/SY
Sample : P5353-03
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E2928

Quant Time: Dec 21 01:39:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Dec 20 23:41:56 2024
Response via : Initial Calibration

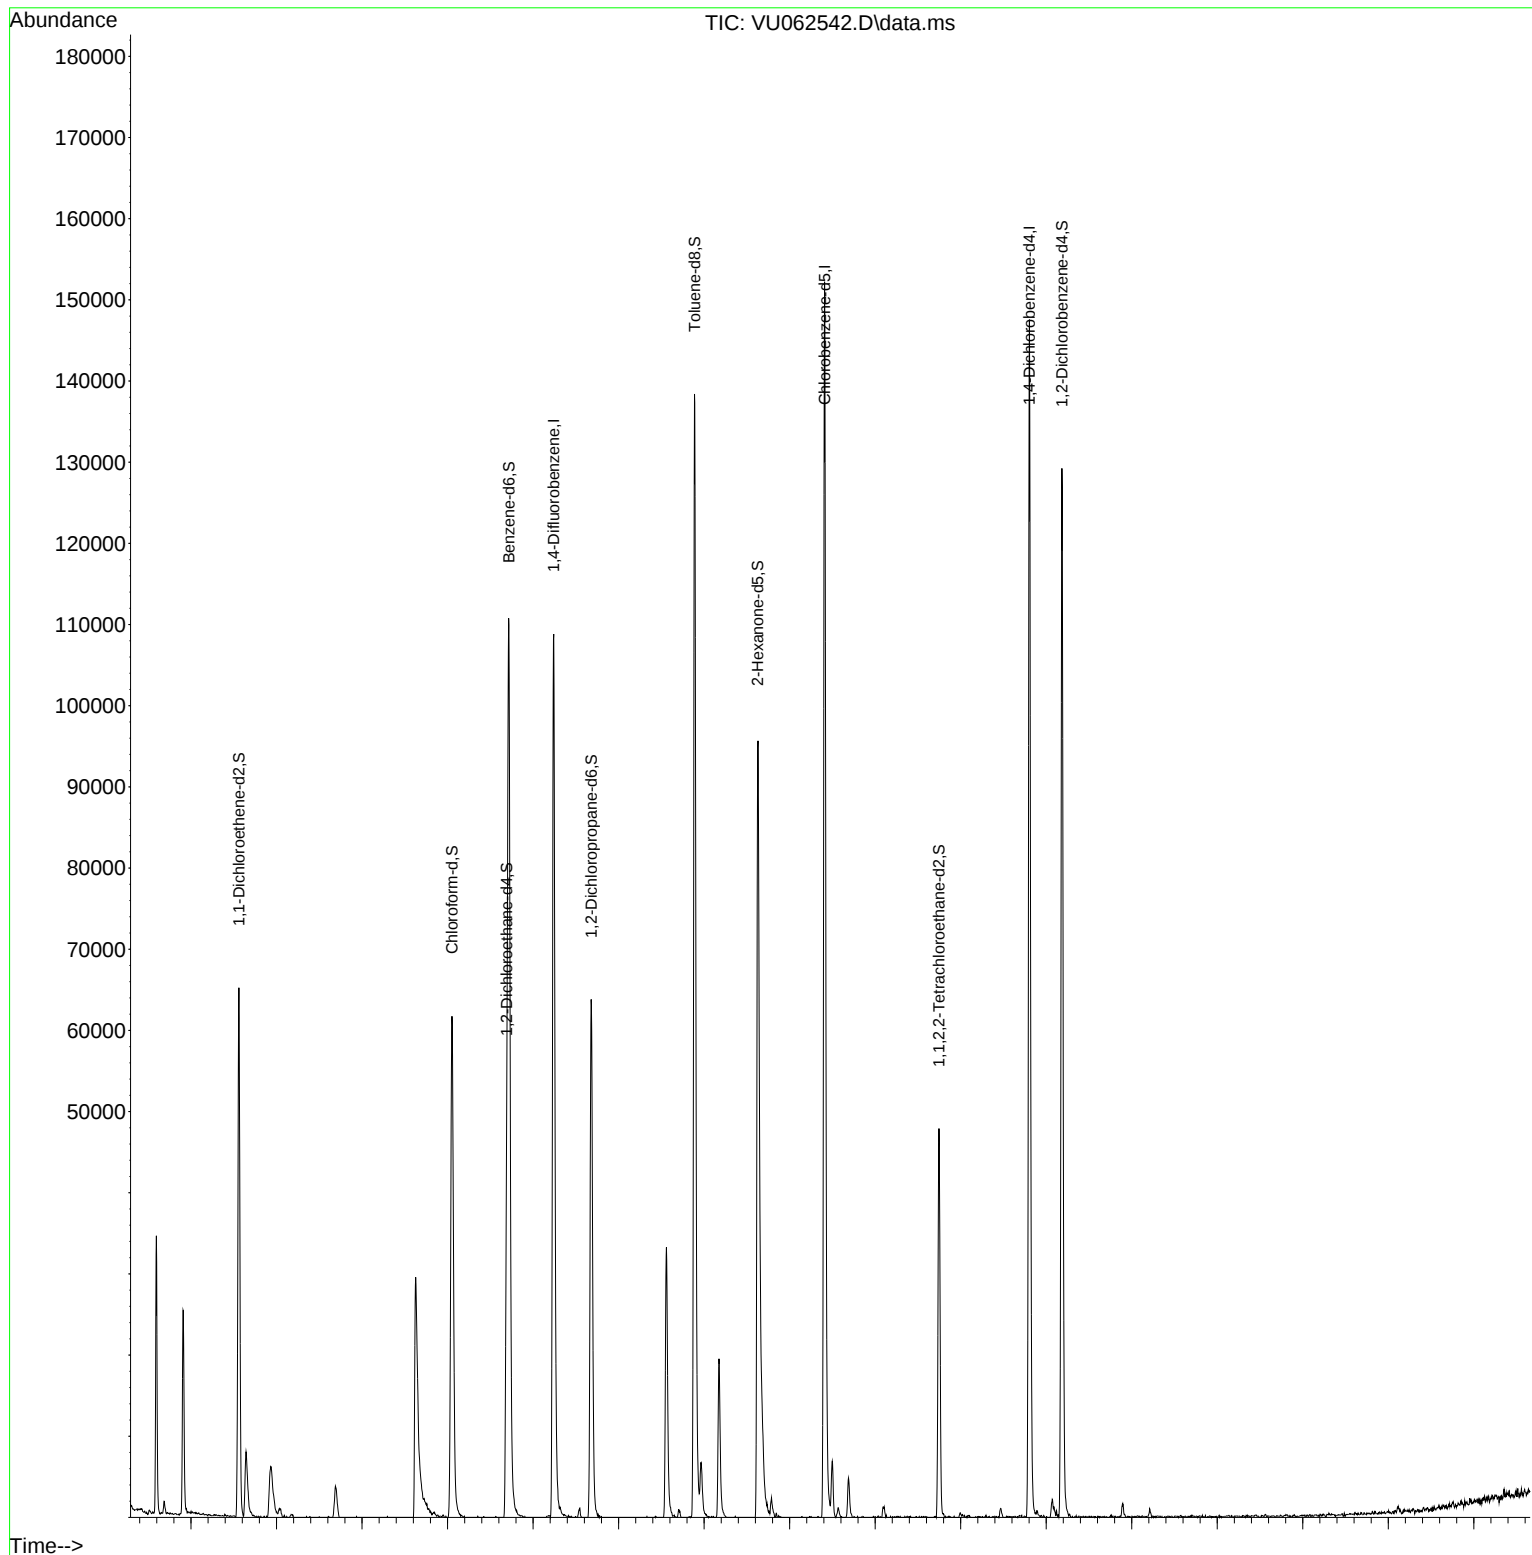

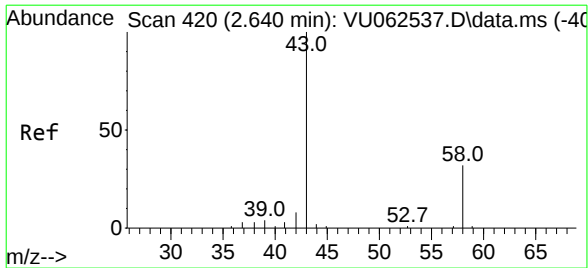

#13
 Acetone
 Concen: 14.271 ug/L
 RT: 2.647 min Scan# 42
 Delta R.T. 0.006 min
 Lab File: VU062542.D
 Acq: 21 Dec 2024 00:04

Instrument :
 MSVOA_U
 ClientSampleId :
 E2928

Tgt Ion: 43 Resp: 11510

Ion	Ratio	Lower	Upper
43	100		
58	34.3	0.0	64.0

