

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122024\
 Data File : VU062543.D
 Acq On : 21 Dec 2024 00:29
 Operator : MD/SY
 Sample : P5353-04
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E2930

Quant Time: Dec 21 01:41:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Dec 20 23:41:56 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	90703	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	85493	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	41233	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	21803	3.564	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	71.200%
7) Chloroethane-d5	1.911	69	18740	4.306	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.200%
11) 1,1-Dichloroethene-d2	2.560	65	11573	3.976	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.600%
20) 2-Butanone-d5	4.628	46	46467	39.631	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	79.260%
24) Chloroform-d	5.052	84	58921	4.450	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.000%
26) 1,2-Dichloroethane-d4	5.692	65	31996	4.914	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.200%
32) Benzene-d6	5.718	84	100756	4.092	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.800%
36) 1,2-Dichloropropane-d6	6.679	67	27427	3.893	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	77.800%
41) Toluene-d8	7.891	98	91263	3.923	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.400%
43) trans-1,3-Dichloroprop...	8.174	79	12337	3.978	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.600%
46) 2-Hexanone-d5	8.627	63	32944	35.213	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	70.420%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	22599	4.122	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.400%
66) 1,2-Dichlorobenzene-d4	12.184	152	35118	4.622	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.400%
Target Compounds					Qvalue	
13) Acetone	2.650	43	11660	14.606	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122024\
Data File : VU062543.D
Acq On : 21 Dec 2024 00:29
Operator : MD/SY
Sample : P5353-04
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E2930

Quant Time: Dec 21 01:41:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Dec 20 23:41:56 2024
Response via : Initial Calibration

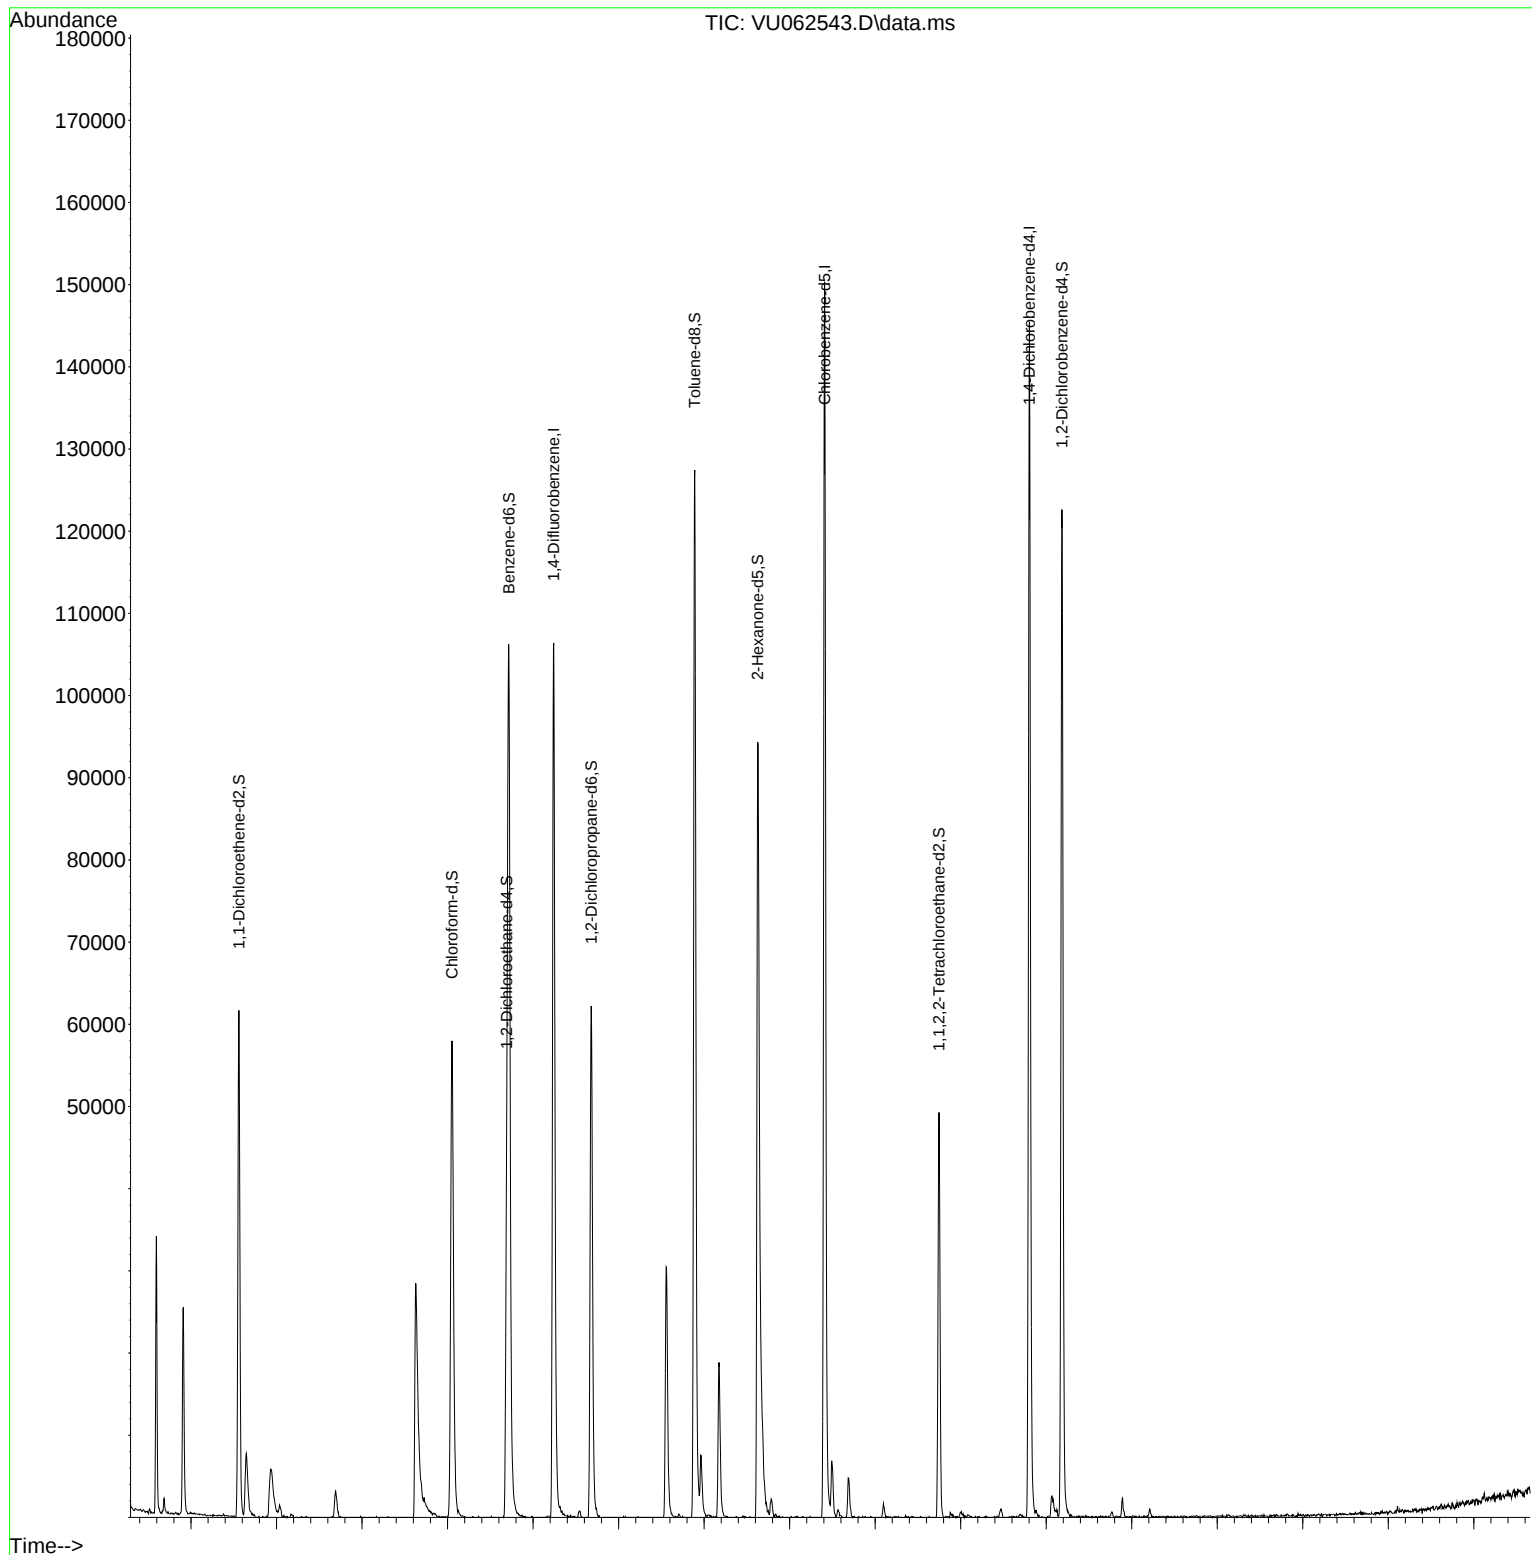

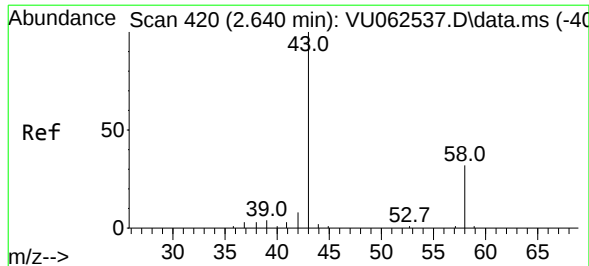

#13

Acetone

Concen: 14.606 ug/L

RT: 2.650 min Scan# 42

Delta R.T. 0.010 min

Lab File: VU062543.D


Acq: 21 Dec 2024 00:29

Instrument :

MSVOA_U

ClientSampleId :

E2930

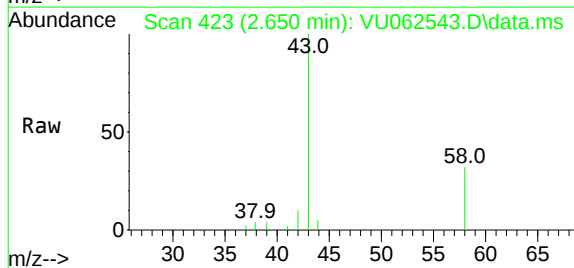

Tgt Ion: 43 Resp: 11660

Ion Ratio Lower Upper

43 100

58 34.0 0.0 64.0

