

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122024\
 Data File : VU062514.D
 Acq On : 20 Dec 2024 10:53
 Operator : MD/SY
 Sample : P5308-08DL 5X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CC8DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU062514.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	110	rVB	42262	47435	12.77%	1.301%
2	1.907	184	192	204	rBV	33669	44669	12.02%	1.225%
3	2.133	252	262	273	rVB	19270	27195	7.32%	0.746%
4	2.560	384	395	410	rBV	81466	133337	35.88%	3.657%
5	3.178	574	587	601	rBV	4041	10060	2.71%	0.276%
6	3.695	738	748	761	rBB3	2271	4751	1.28%	0.130%
7	4.628	1024	1038	1064	rBV	41877	117307	31.57%	3.218%
8	5.052	1156	1170	1205	rBV	76702	173475	46.68%	4.758%
9	5.714	1358	1376	1415	rBV2	138230	366262	98.56%	10.046%
10	6.238	1528	1539	1563	rBV	154223	299261	80.53%	8.208%
11	6.534	1619	1631	1661	rBV	124247	239737	64.52%	6.576%
12	6.682	1664	1677	1699	rVB	82147	163543	44.01%	4.486%
13	7.557	1939	1949	1976	rBV	44757	82171	22.11%	2.254%
14	7.891	2041	2053	2073	rBV	181050	320812	86.33%	8.800%
15	8.174	2131	2141	2156	rBV3	25245	45510	12.25%	1.248%
16	8.544	2245	2256	2273	rBV2	113269	198004	53.28%	5.431%
17	8.627	2273	2282	2319	rVV2	126244	286037	76.98%	7.846%
18	9.409	2514	2525	2554	rBV	215431	371597	100.00%	10.193%
19	10.746	2931	2941	2962	rBB	62717	102096	27.47%	2.800%
20	11.804	3259	3270	3291	rBV	205861	338131	90.99%	9.275%
21	12.184	3377	3388	3415	rBV	161378	274376	73.84%	7.526%




Sum of corrected areas: 3645766

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122024\
Data File : VU062514.D
Acq On : 20 Dec 2024 10:53
Operator : MD/SY
Sample : P5308-08DL 5X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CC8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

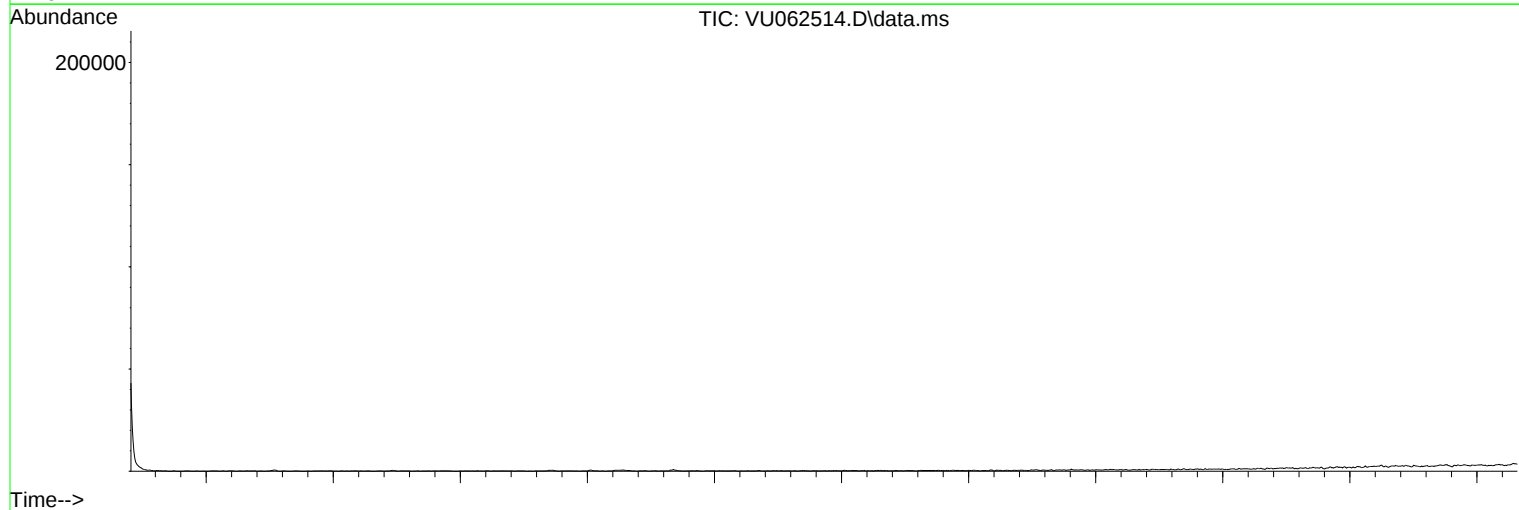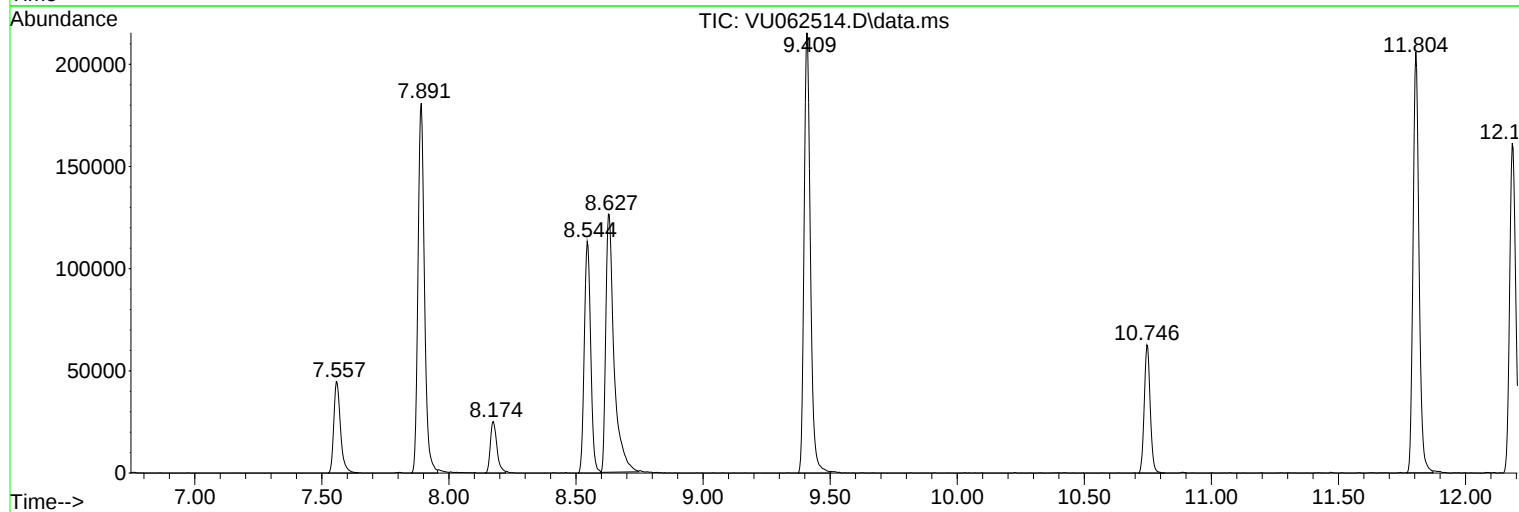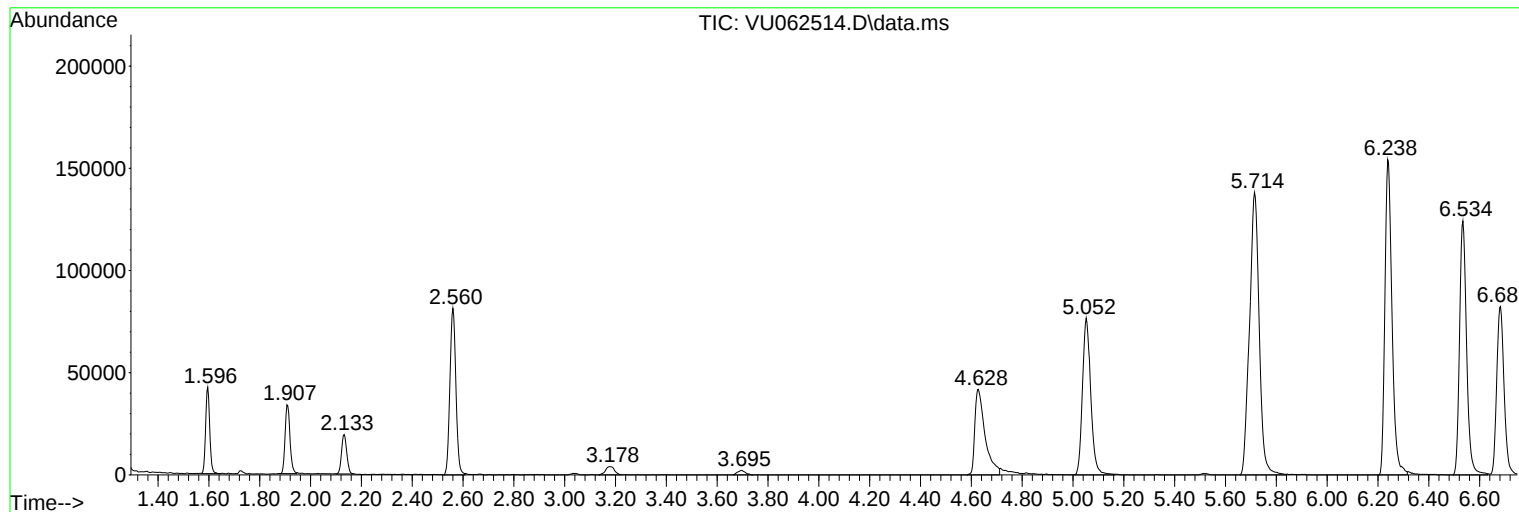

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122024\
Data File : VU062514.D
Acq On : 20 Dec 2024 10:53
Operator : MD/SY
Sample : P5308-08DL 5X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CC8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122024\
Data File : VU062514.D
Acq On : 20 Dec 2024 10:53
Operator : MD/SY
Sample : P5308-08DL 5X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CC8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------