

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122024\
 Data File : VU062515.D
 Acq On : 20 Dec 2024 11:17
 Operator : MD/SY
 Sample : P5308-10DL 10X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CD1DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU062515.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	86	94	114	rVB	36779	44568	11.29%	1.365%
2	1.907	184	192	205	rBV	28859	40755	10.33%	1.249%
3	2.071	235	243	253	rVB2	3474	4782	1.21%	0.147%
4	2.557	382	394	415	rVB	76201	123594	31.32%	3.787%
5	3.174	572	586	604	rBV2	12276	28926	7.33%	0.886%
6	3.689	736	746	760	rBB3	4018	8191	2.08%	0.251%
7	4.634	1024	1040	1073	rBV5	43891	159577	40.44%	4.889%
8	5.052	1155	1170	1195	rBV	69430	156871	39.76%	4.806%
9	5.714	1358	1376	1399	rBV2	128249	331058	83.90%	10.143%
10	6.238	1528	1539	1559	rBV	122599	237291	60.14%	7.270%
11	6.531	1618	1630	1653	rBV	206232	394583	100.00%	12.089%
12	6.679	1664	1676	1696	rVB2	76192	148038	37.52%	4.535%
13	7.557	1938	1949	1969	rBV	39179	71653	18.16%	2.195%
14	7.888	2041	2052	2072	rBV	161275	286610	72.64%	8.781%
15	8.174	2131	2141	2160	rBV2	22997	40991	10.39%	1.256%
16	8.547	2248	2257	2267	rBB2	10574	17076	4.33%	0.523%
17	8.631	2273	2283	2320	rBV3	120958	268884	68.14%	8.238%
18	9.409	2511	2525	2548	rBV	168834	287520	72.87%	8.809%
19	10.746	2931	2941	2959	rBB	57153	93642	23.73%	2.869%
20	11.804	3257	3270	3294	rBV	163223	266341	67.50%	8.160%
21	12.183	3377	3388	3409	rBV	147877	253090	64.14%	7.754%

Sum of corrected areas: 3264041




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122024\
Data File : VU062515.D
Acq On : 20 Dec 2024 11:17
Operator : MD/SY
Sample : P5308-10DL 10X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CD1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

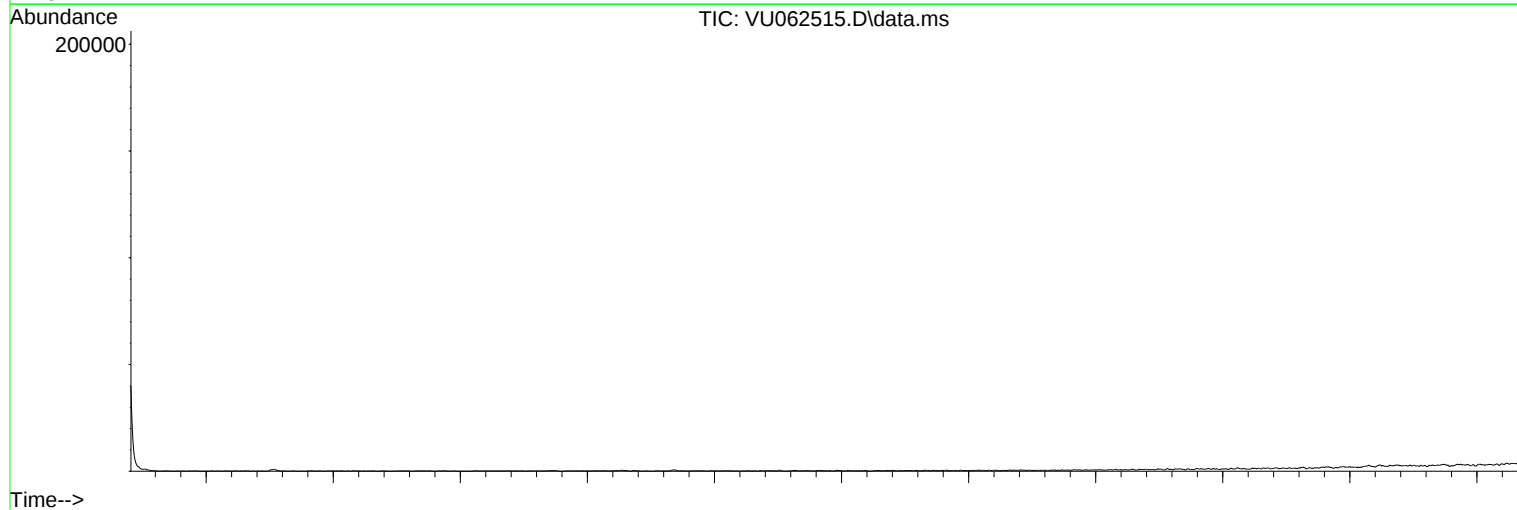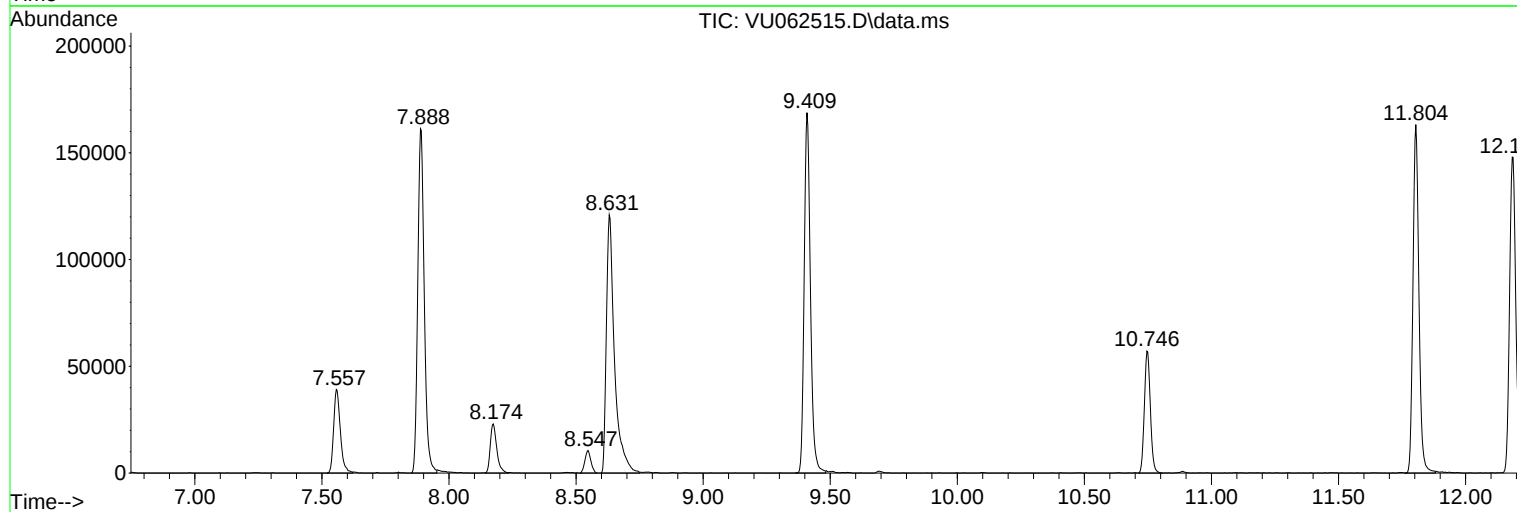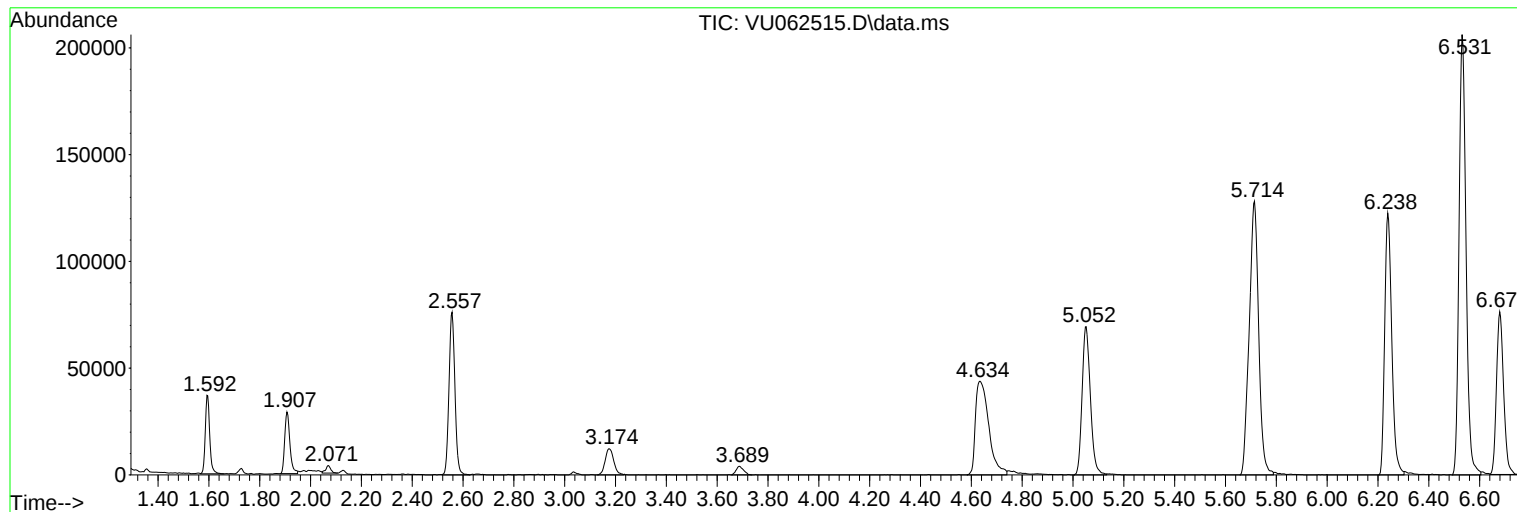

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122024\
Data File : VU062515.D
Acq On : 20 Dec 2024 11:17
Operator : MD/SY
Sample : P5308-10DL 10X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CD1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122024\
Data File : VU062515.D
Acq On : 20 Dec 2024 11:17
Operator : MD/SY
Sample : P5308-10DL 10X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CD1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------