

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U122319\
 Data File : VU036332.D
 Acq On : 23 Dec 2019 17:36
 Operator : JC/MD
 Sample : K6282-21
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Quant Time: Dec 24 01:39:02 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 24 00:19:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	260407	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	285620	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	118864	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	133395	5.82	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	116.40%
7) Chloroethane-d5	1.93	69	114662	5.58	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.60%
11) 1,1-Dichloroethene-d2	2.59	63	137097	4.14	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.80%
20) 2-Butanone-d5	4.69	46	221035	51.45	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.90%
24) Chloroform-d	5.11	84	187296	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.60%
26) 1,2-Dichloroethane-d4	5.75	65	102036	5.27	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.40%
32) Benzene-d6	5.77	84	371905	5.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.60%
36) 1,2-Dichloropropane-d6	6.73	67	113203	5.01	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.20%
41) Toluene-d8	7.93	98	309441	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.60%
43) trans-1,3-Dichloropropene-	8.21	79	43448	4.67	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.40%
46) 2-Hexanone-d5	8.68	63	175155	49.21	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.42%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	99509	4.81	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.20%
64) 1,2-Dichlorobenzene-d4	12.22	152	122668	5.39	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.80%


Target Compounds				Ovalue
13) Acetone	2.68	43	9775	2.611 ug/L 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU122319\
Data File : VU036332.D
Acq On : 23 Dec 2019 17:36
Operator : JC/MD
Sample : K6282-21
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Time: Dec 24 01:39:02 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 24 00:19:34 2019
Response via : Initial Calibration

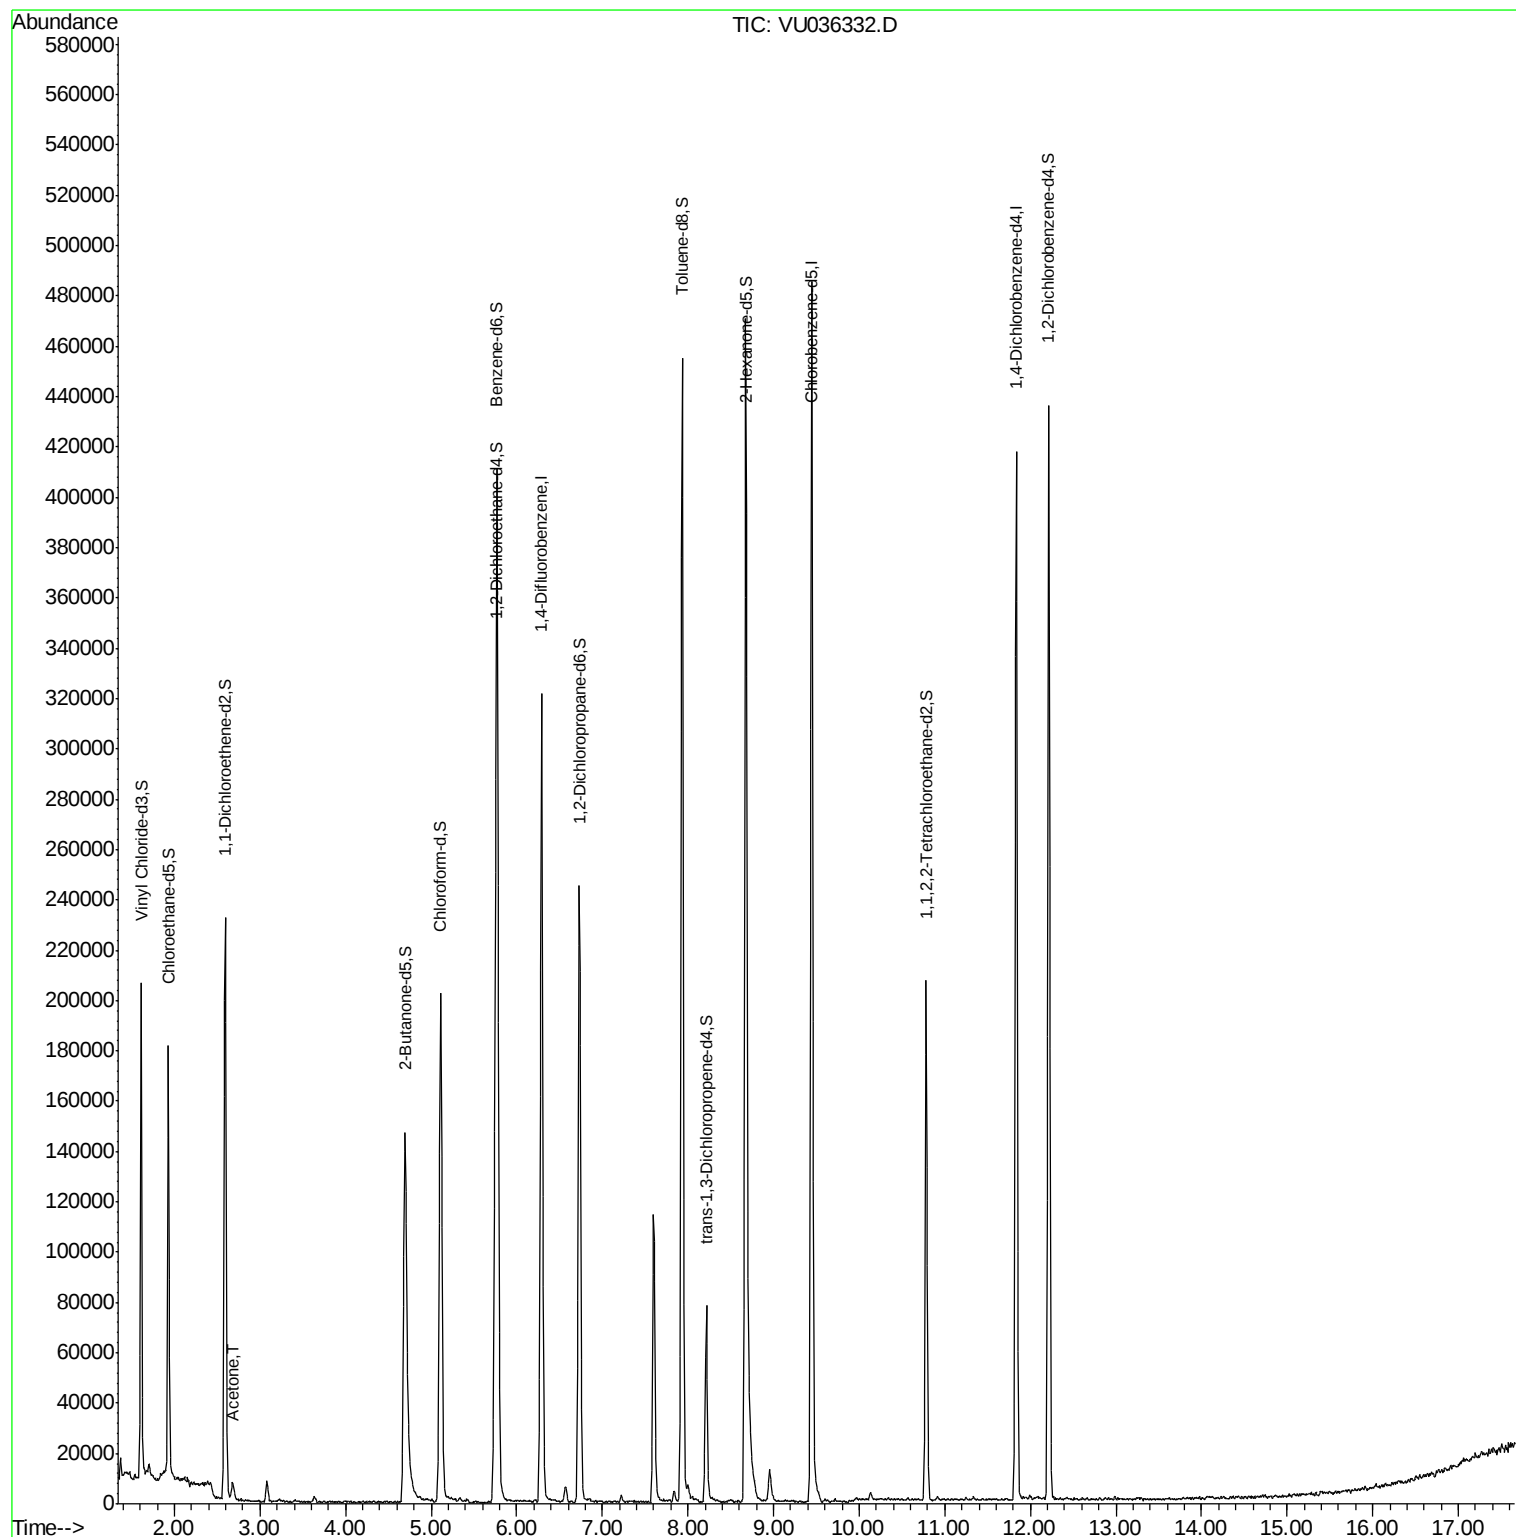

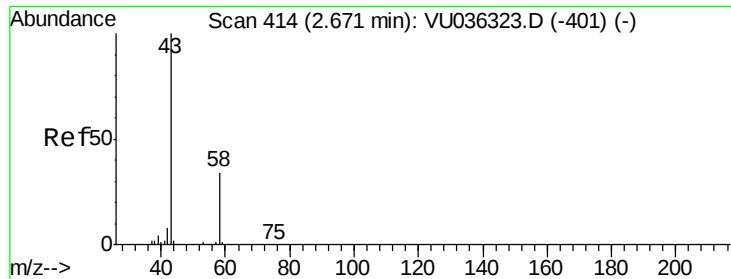

#13

Acetone

Concen: 2.611 ug/L

RT: 2.68 min Scan# 416

Delta R.T. 0.01 min

Lab File: VU036332.D

Acq: 23 Dec 2019 17:36

Instrument :

MSVOA_U

ClientSampleId :

VHBLK01

Tot Ion: 43 Resp: 9775

Ion Ratio Lower Upper

43 100

58 31.6 0.0 67.6

