


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU122319\
Data File : VU036322.D
Acq On : 23 Dec 2019 09:00
Operator : JC/MD
Sample : BFB24
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB24

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121319WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Dec 24 01:02:46 2019

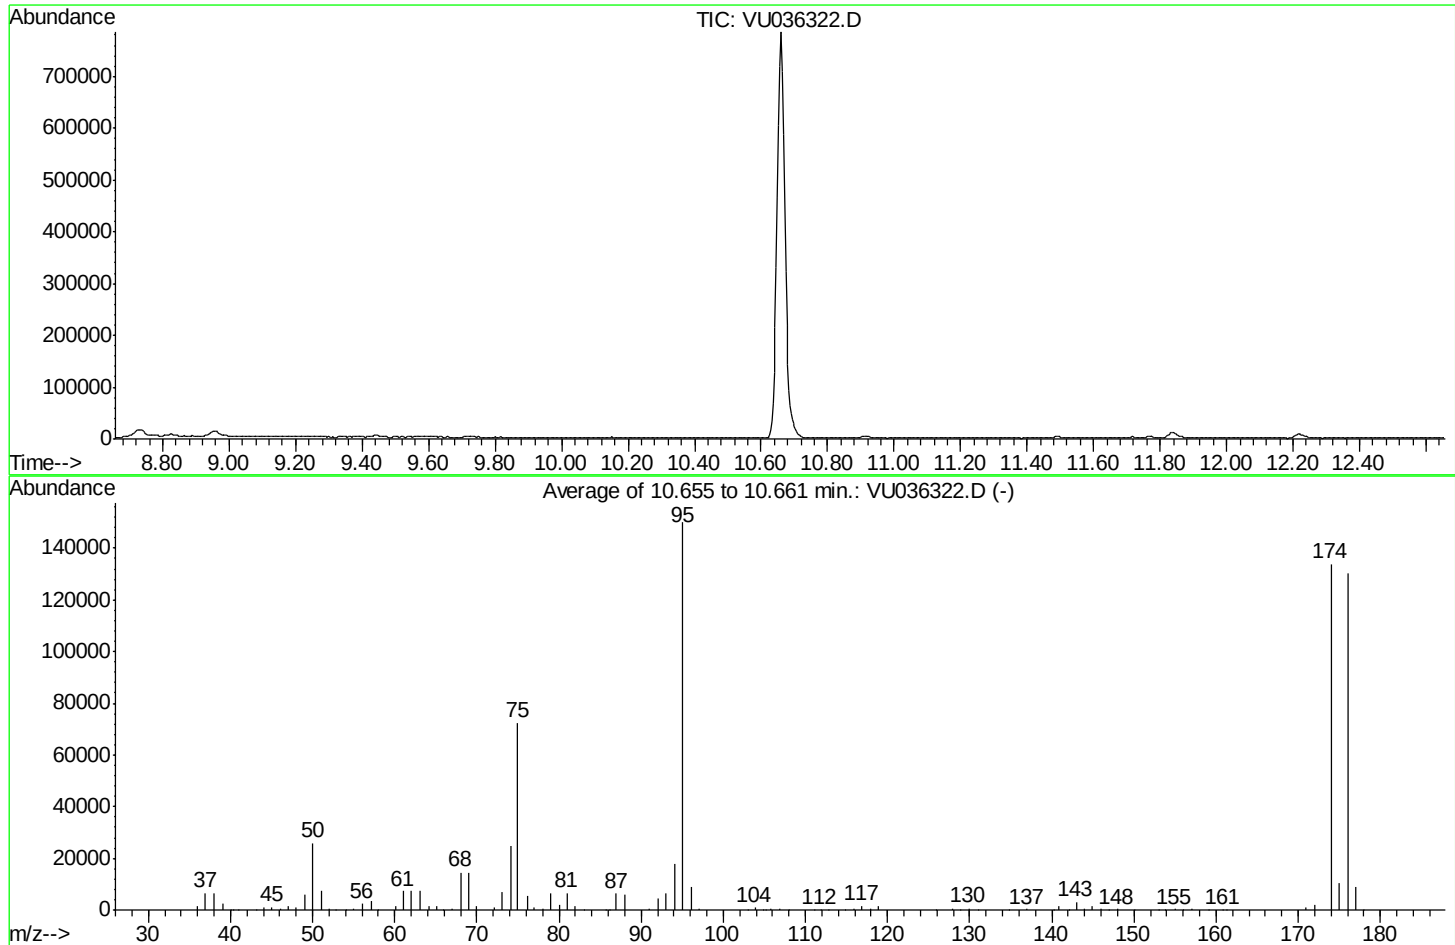

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	25840	PASS
75	95	30	80	48.2	72344	PASS
95	95	100	100	100.0	150016	PASS
96	95	5	9	6.0	8996	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	89.2	133773	PASS
175	174	5	9	7.8	10500	PASS
176	174	95	101	97.5	130394	PASS
177	176	5	9	6.8	8844	PASS

Scan 2883 (10.610 min): VU036322.D
BFB24

m/z	Abundance
36.00	968.0
36.80	109.0
37.90	351.0
39.80	102.0
43.90	359.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

m/z	Abundance
36.00	2341.0
37.00	6334.0
38.00	6572.0
39.10	2687.0
40.00	248.0
40.90	154.0
44.10	1282.0
45.10	914.0
46.20	330.0
47.00	1313.0
48.00	876.0
49.10	5922.0
50.00	24040.0
51.10	7086.0
52.00	388.0
52.90	231.0
54.00	121.0
55.10	411.0
56.00	2211.0
57.10	3242.0
58.00	227.0
60.00	1292.0
61.00	6729.0
62.00	7395.0
63.10	6796.0
64.10	1343.0
65.10	1551.0
66.00	146.0
67.00	473.0
68.00	13124.0
69.10	13685.0
70.00	1357.0
72.10	884.0
73.10	6779.0
74.10	24056.0
75.00	70040.0
76.10	5372.0
77.00	815.0
78.00	763.0
78.90	6406.0
80.00	2093.0
81.00	6244.0
82.00	1342.0
82.90	198.0
85.60	265.0
86.90	6336.0
88.00	5297.0
91.00	574.0
92.00	4073.0
93.00	6175.0
94.10	17008.0
95.10	141440.0
96.10	8861.0
97.00	273.0
103.00	132.0
103.90	745.0
104.80	169.0
105.20	176.0
105.90	633.0
106.90	263.0
111.90	179.0
112.80	135.0
116.00	715.0
116.90	1509.0
117.90	618.0
118.90	1412.0
127.90	495.0
128.80	249.0
129.90	622.0
130.90	170.0
134.80	250.0
137.00	343.0
140.80	1301.0
142.10	233.0
143.00	3002.0
144.10	264.0
144.90	1535.0
146.00	303.0
148.00	329.0
153.00	252.0
153.80	103.0
154.90	315.0
157.00	310.0
159.00	169.0
160.80	142.0
161.20	105.0
171.00	1079.0
172.00	1743.0
174.00	125864.0
175.00	9589.0
176.00	119888.0
177.00	8443.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

177.90

233.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

m/z	Abundance
36.00	2310.0
37.00	6910.0
38.00	6728.0
39.00	2729.0
40.10	215.0
40.90	122.0
43.20	117.0
44.10	1281.0
45.00	1010.0
46.20	331.0
47.00	1497.0
48.00	992.0
49.10	6270.0
50.00	26880.0
51.10	7779.0
52.00	403.0
52.80	237.0
54.10	215.0
55.00	362.0
56.00	2389.0
57.10	3620.0
58.00	230.0
60.00	1433.0
61.00	7553.0
62.00	7505.0
63.10	7405.0
64.10	1632.0
65.10	1465.0
66.00	184.0
67.10	486.0
68.10	15121.0
69.00	14618.0
70.00	1261.0
72.10	920.0
73.10	7228.0
74.10	25616.0
75.00	74312.0
76.10	5672.0
77.00	902.0
78.00	774.0
78.90	6617.0
80.00	2198.0
81.00	6729.0
82.00	1508.0
82.90	242.0
85.70	188.0
86.10	211.0
87.00	6424.0
88.00	6045.0
91.00	599.0
92.00	4500.0
93.00	6728.0
94.00	18232.0
95.10	154496.0
96.10	9257.0
97.00	319.0
103.00	135.0
103.90	782.0
105.10	173.0
105.80	655.0
106.90	338.0
111.00	195.0
111.90	187.0
114.90	114.0
115.90	763.0
116.90	1638.0
117.90	644.0
118.90	1472.0
126.00	127.0
128.00	548.0
128.80	228.0
129.90	696.0
130.90	234.0
134.80	226.0
137.00	383.0
140.90	1549.0
142.10	268.0
143.00	3253.0
144.00	281.0
144.90	1668.0
146.10	298.0
147.90	365.0
153.00	196.0
153.80	132.0
154.90	429.0
155.90	111.0
157.00	413.0
159.00	188.0
160.80	176.0
161.20	133.0
170.90	1159.0
171.90	1961.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

174.00	137856.0
175.00	10875.0
176.00	134720.0
177.00	9019.0
177.90	251.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

m/z	Abundance
36.00	2127.0
37.00	6822.0
38.00	6417.0
39.00	2743.0
40.30	295.0
43.10	124.0
44.00	1244.0
45.10	1085.0
46.10	254.0
47.00	1632.0
48.00	964.0
49.10	5789.0
50.10	26600.0
51.10	7852.0
52.00	346.0
52.90	226.0
54.10	239.0
54.90	341.0
56.00	2287.0
57.10	3634.0
58.00	196.0
60.10	1383.0
61.00	7640.0
62.00	6880.0
63.00	7482.0
64.10	1731.0
65.10	1350.0
65.90	220.0
68.10	15285.0
69.00	14431.0
70.00	1257.0
72.10	857.0
73.00	7039.0
74.10	25408.0
75.00	72680.0
76.10	5528.0
77.00	913.0
78.10	672.0
78.90	6453.0
80.00	2067.0
81.00	6534.0
82.00	1544.0
83.00	244.0
86.10	333.0
87.00	6348.0
88.00	6311.0
90.90	605.0
92.00	4621.0
93.00	6899.0
94.00	18064.0
95.10	154112.0
96.10	8871.0
97.00	297.0
103.90	789.0
105.00	162.0
105.80	670.0
106.90	295.0
107.90	154.0
111.00	252.0
111.80	188.0
114.80	148.0
115.90	697.0
116.90	1502.0
117.90	623.0
118.90	1310.0
125.90	165.0
128.00	520.0
128.90	183.0
129.90	774.0
131.00	216.0
134.80	215.0
136.90	341.0
140.20	147.0
140.90	1525.0
142.10	238.0
143.00	3388.0
143.90	286.0
144.90	1680.0
146.10	233.0
146.90	107.0
147.90	391.0
150.00	116.0
152.90	106.0
153.80	111.0
155.00	558.0
155.90	146.0
157.00	463.0
159.00	218.0
160.90	191.0
170.90	1023.0
171.90	2135.0
174.00	137600.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

175.00	11037.0
176.00	136576.0
177.00	9071.0
177.90	270.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24